

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.


Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS


**IMAGES ARE BEST AVAILABLE COPY.**

As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.

FIG. 1

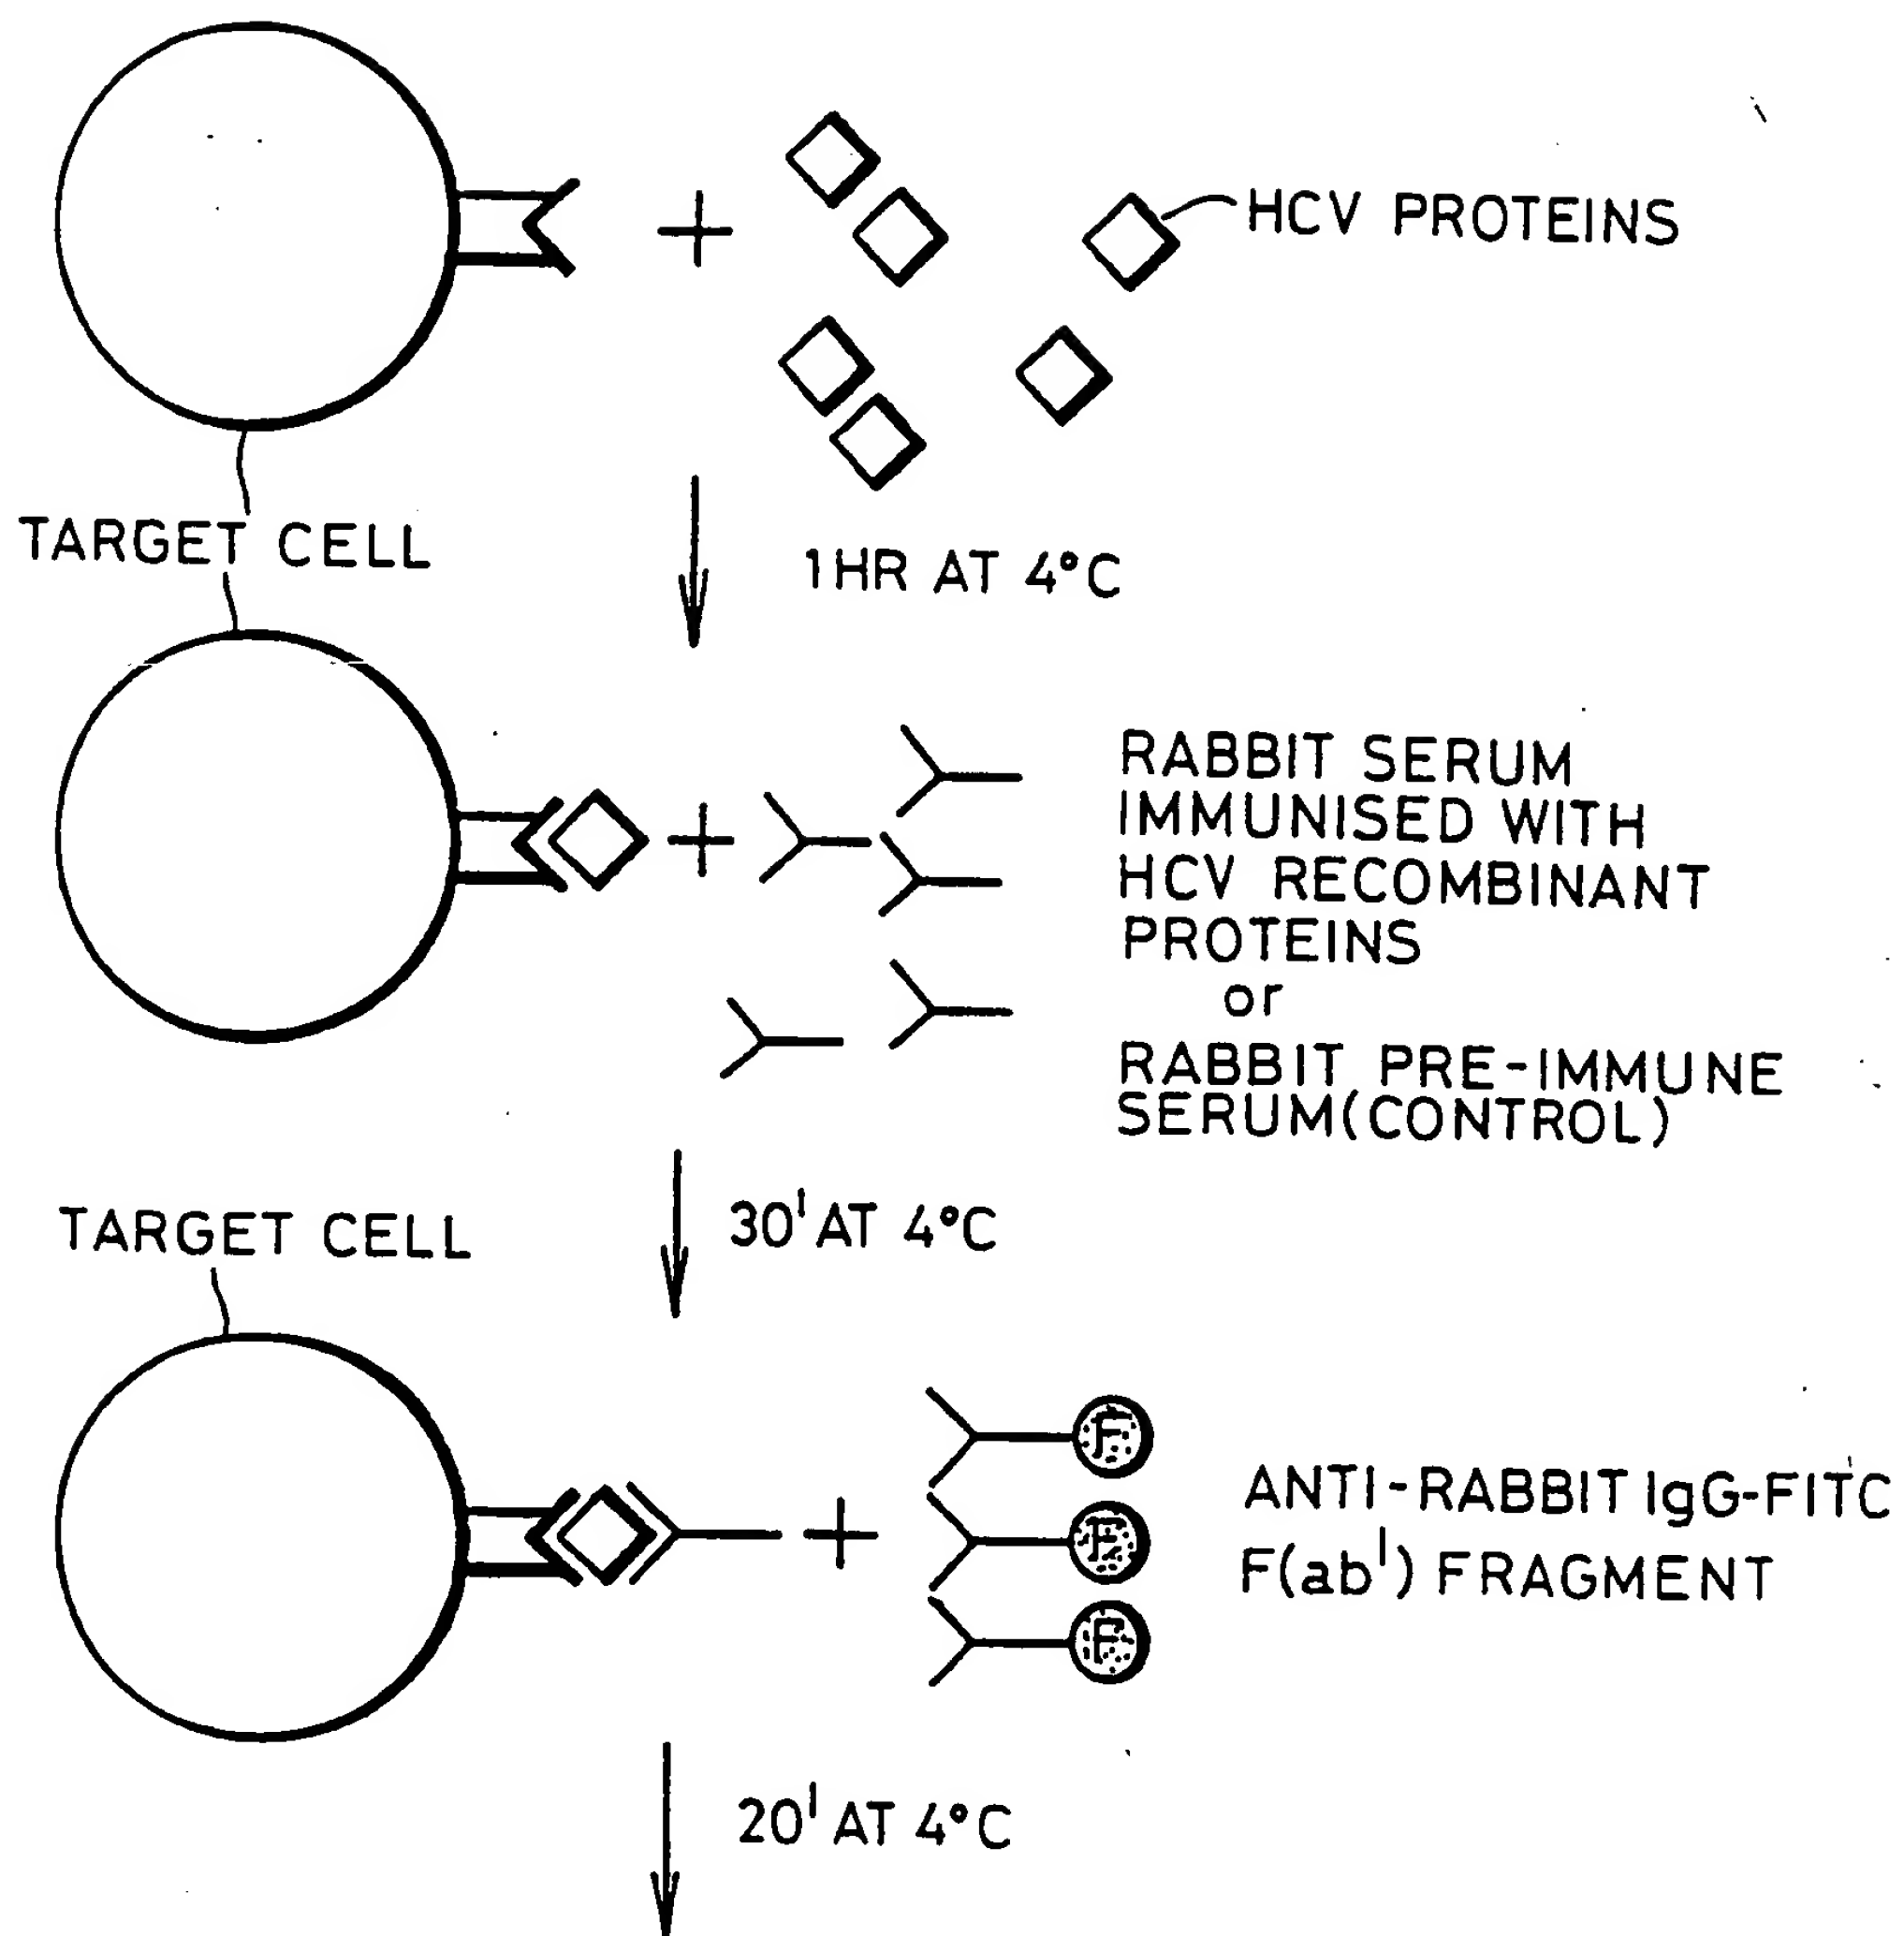

FACScan ANALYSIS

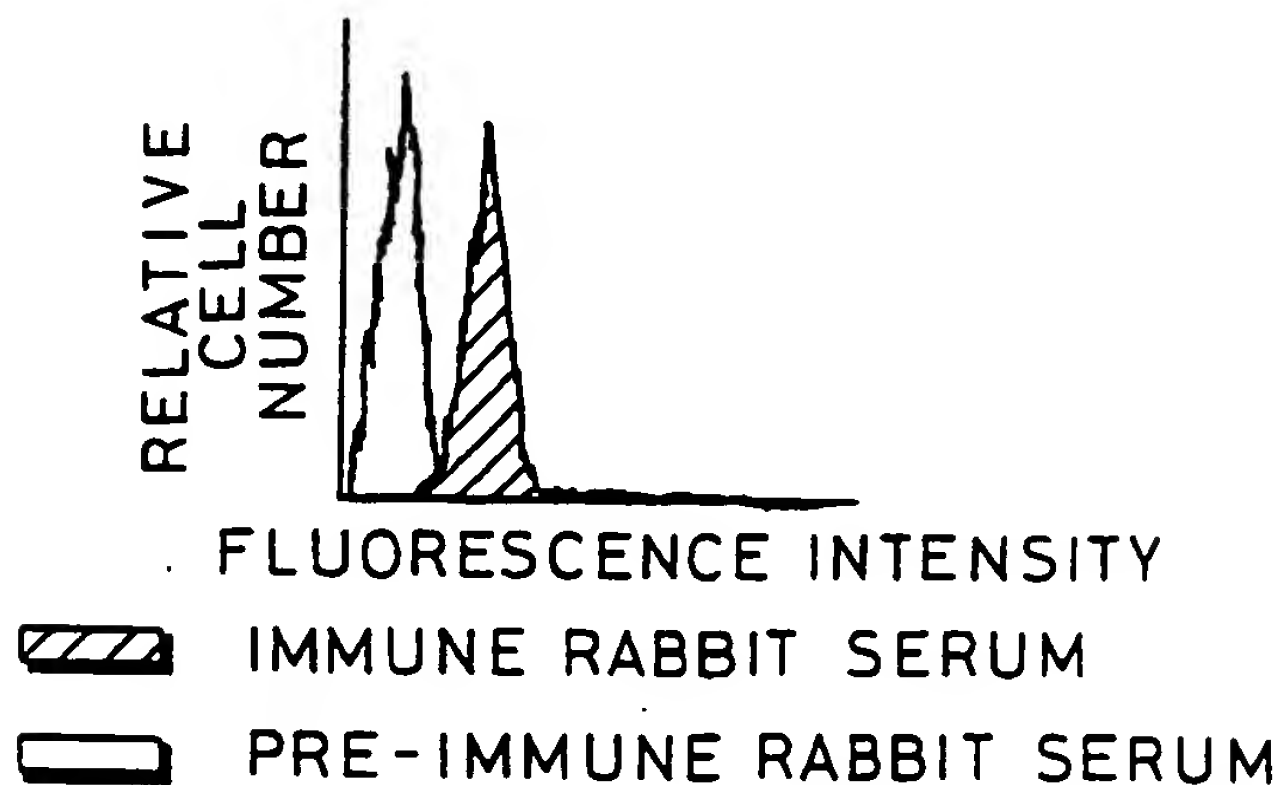

2/14

FIG. 2(A)

MOLT 4


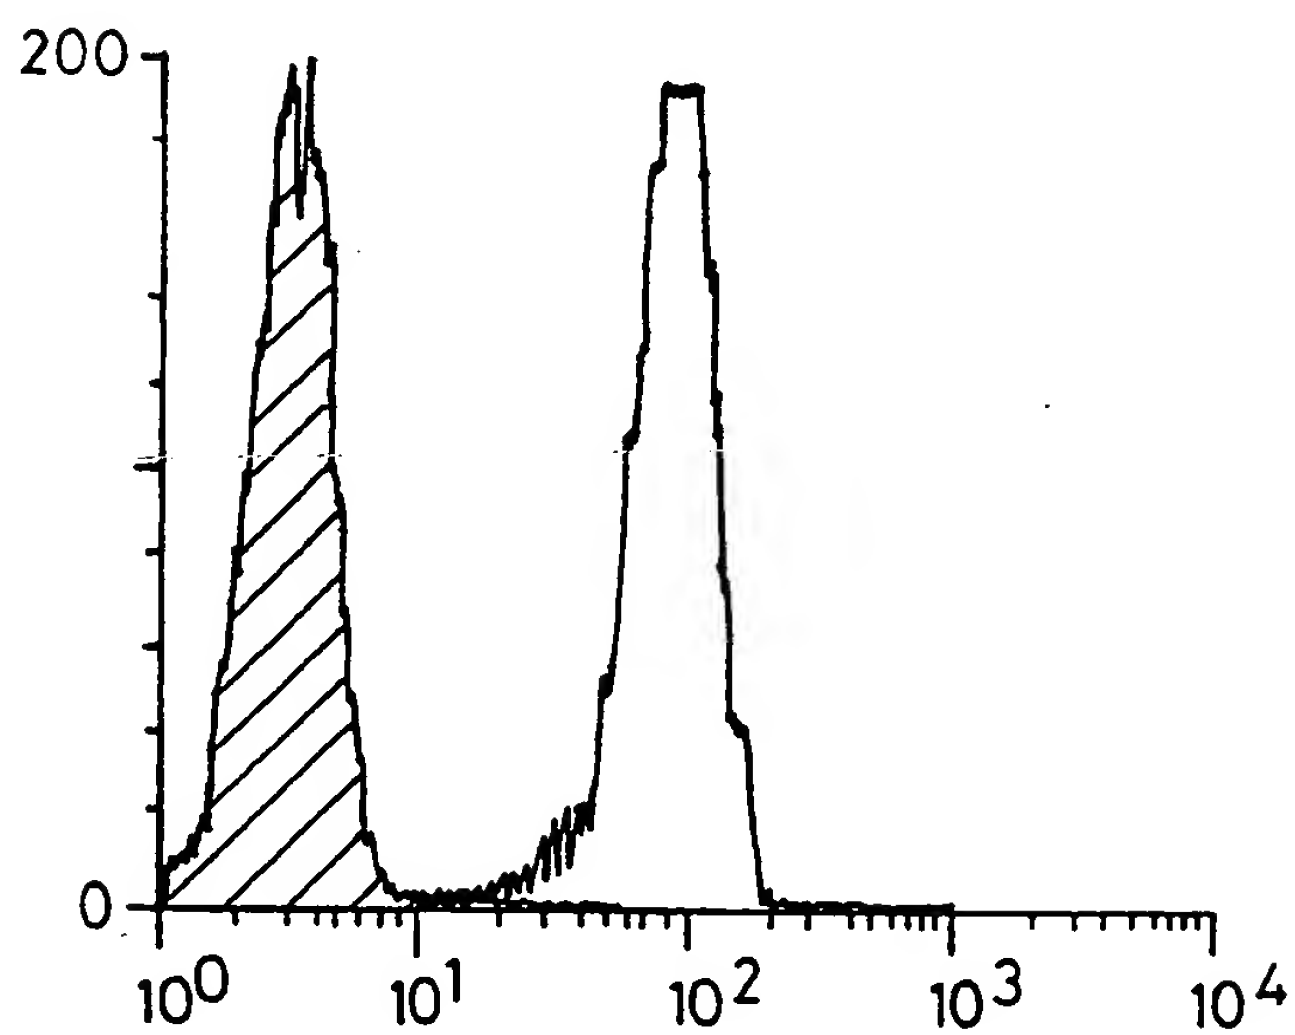


FIG. 2(B)

JURKAT

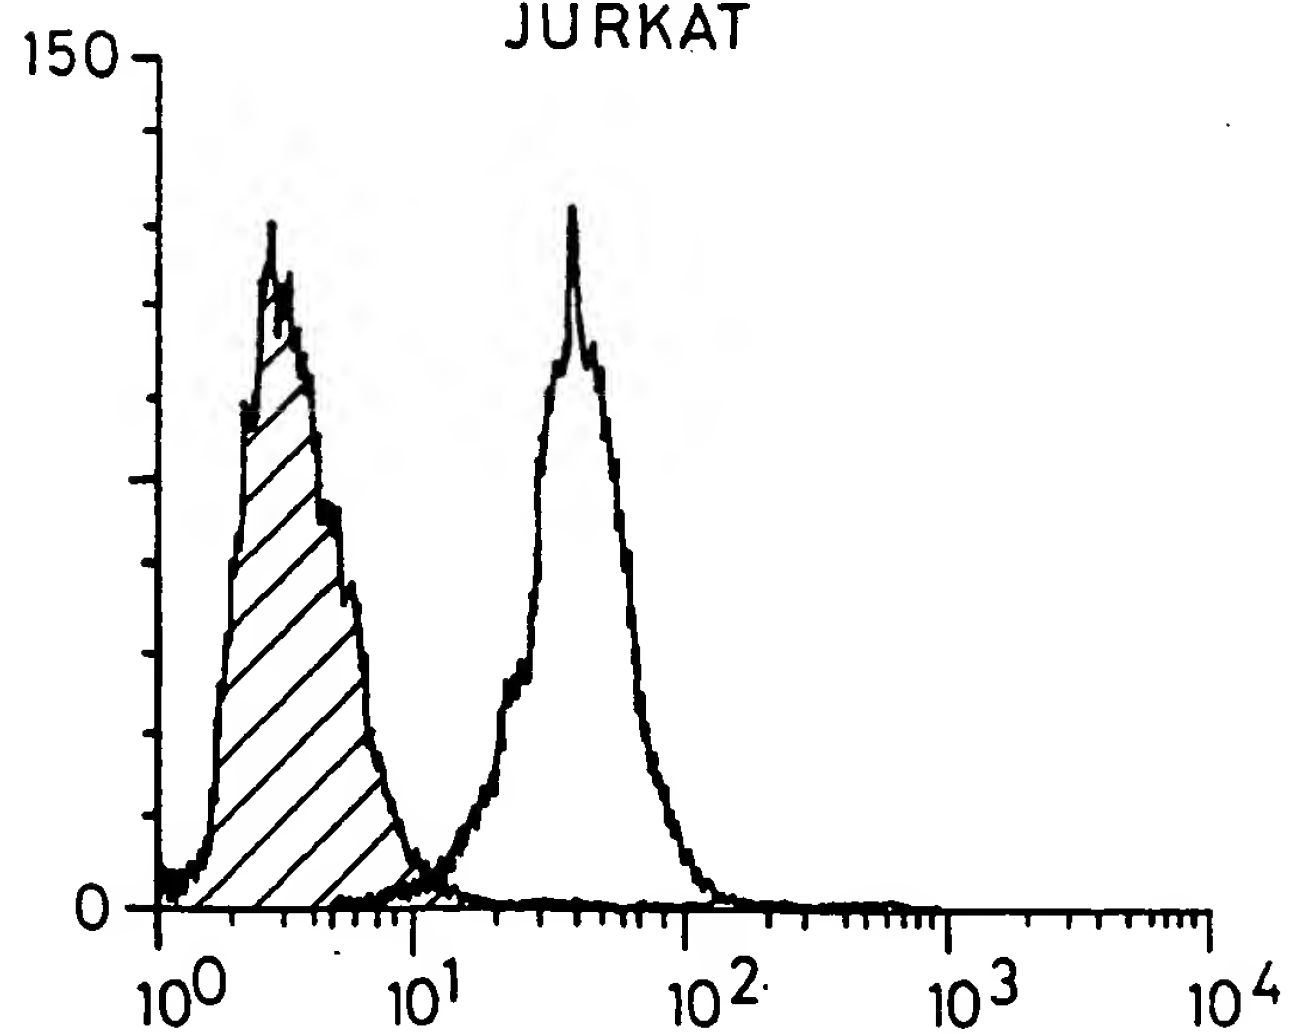

3/14

FIG. 2(C)

K562


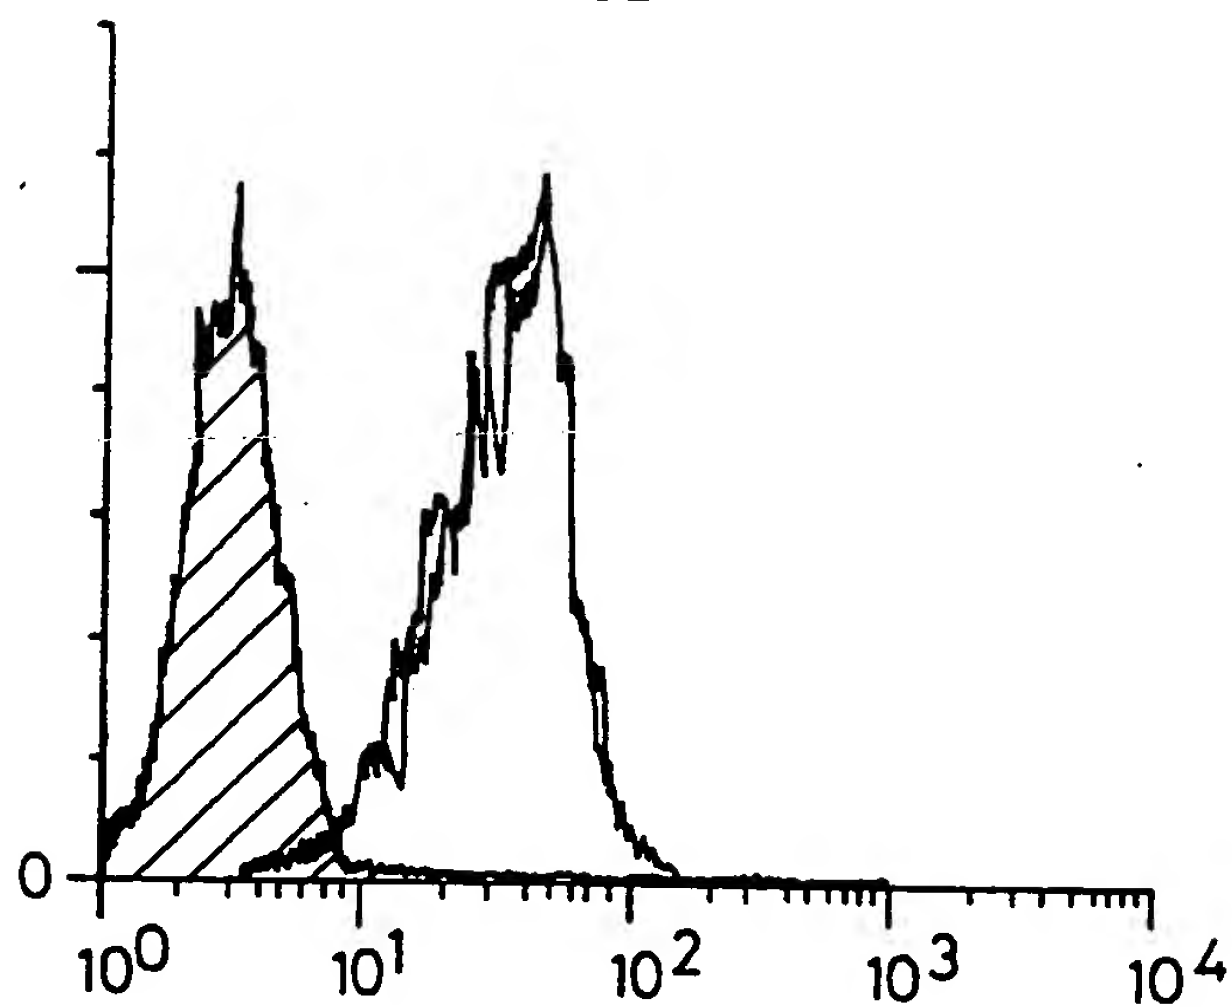


FIG. 2(D)

EBV-B

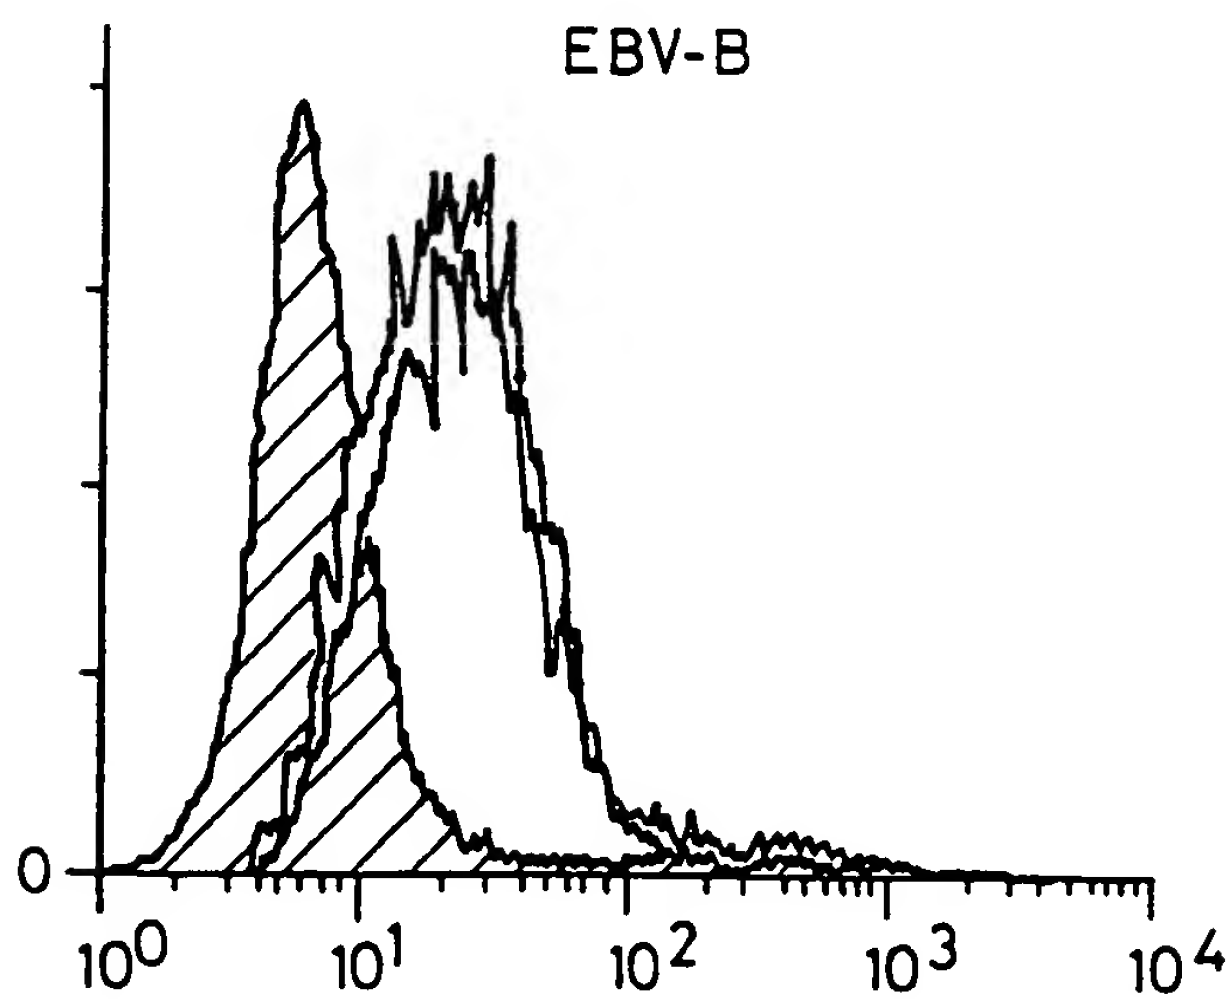

4/14

FIG. 2(E)

DAUDI


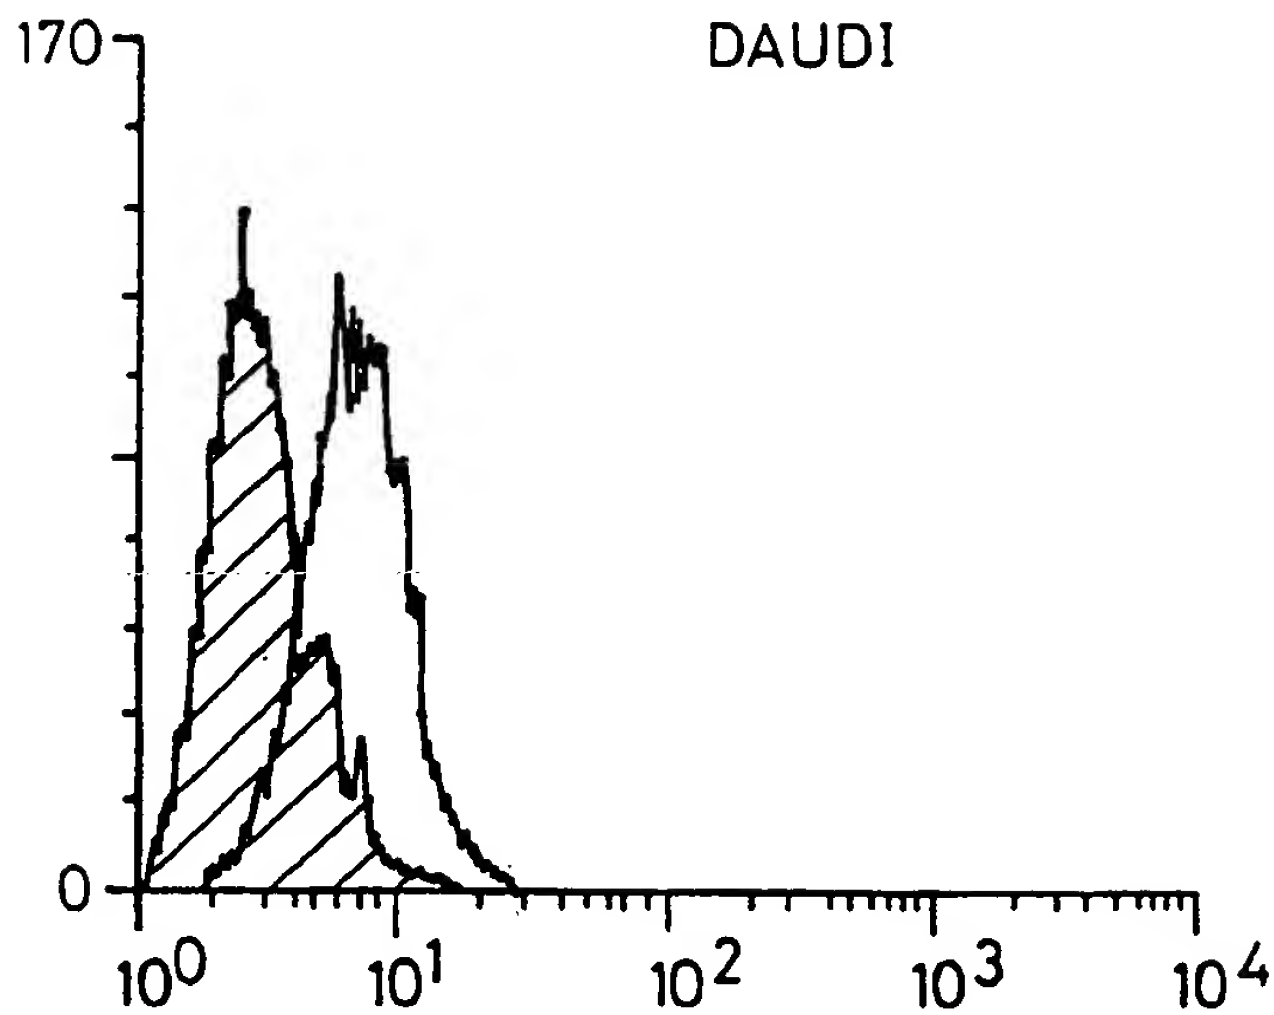


FIG. 2(F)

HELA

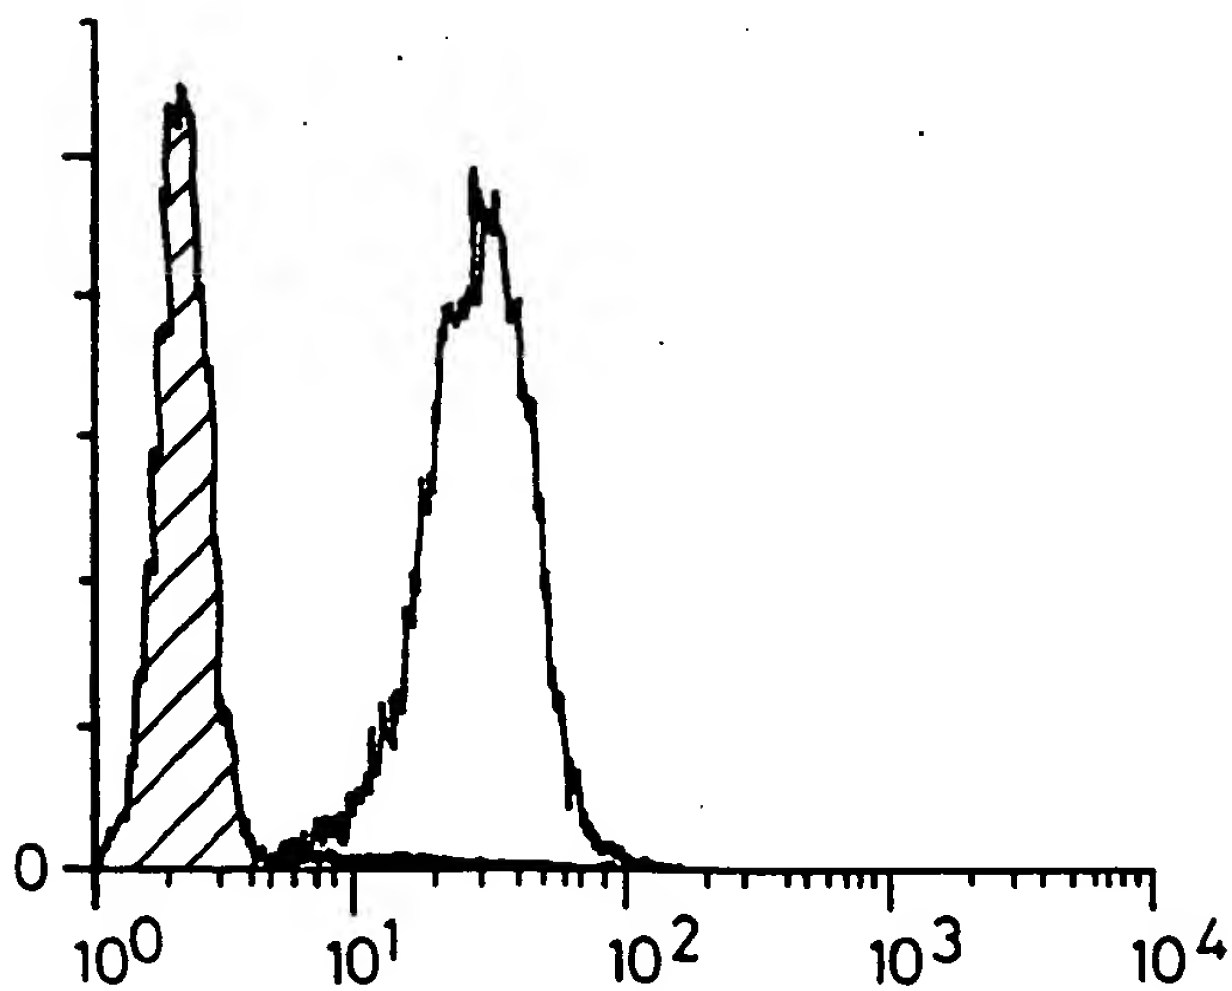

5/14

FIG. 2(G)  
ADENOCARCINOMA


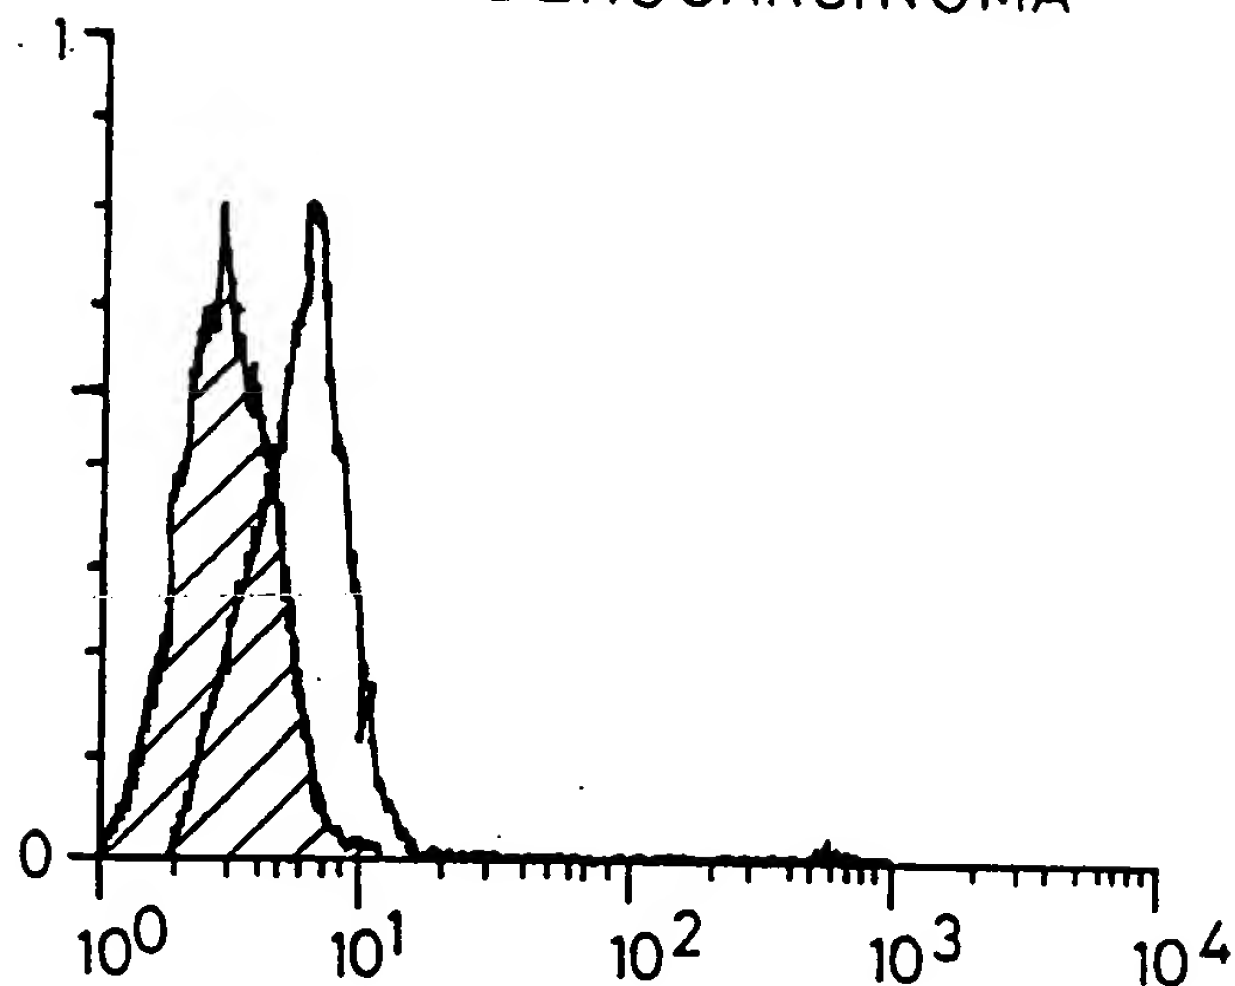


FIG. 2(H)  
HUH 7

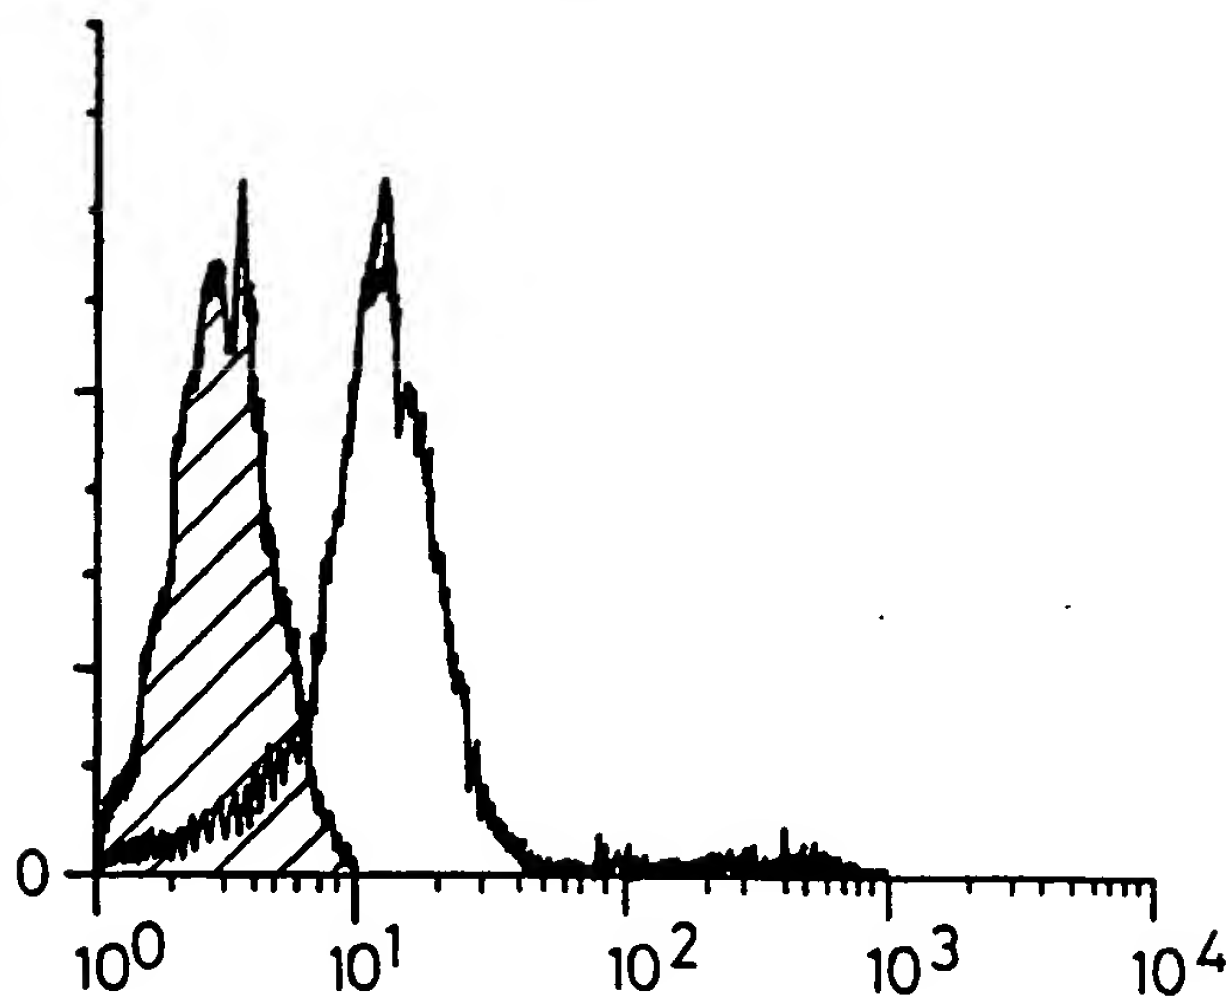

6/14

FIG. 3(A)

PURIFIED RA


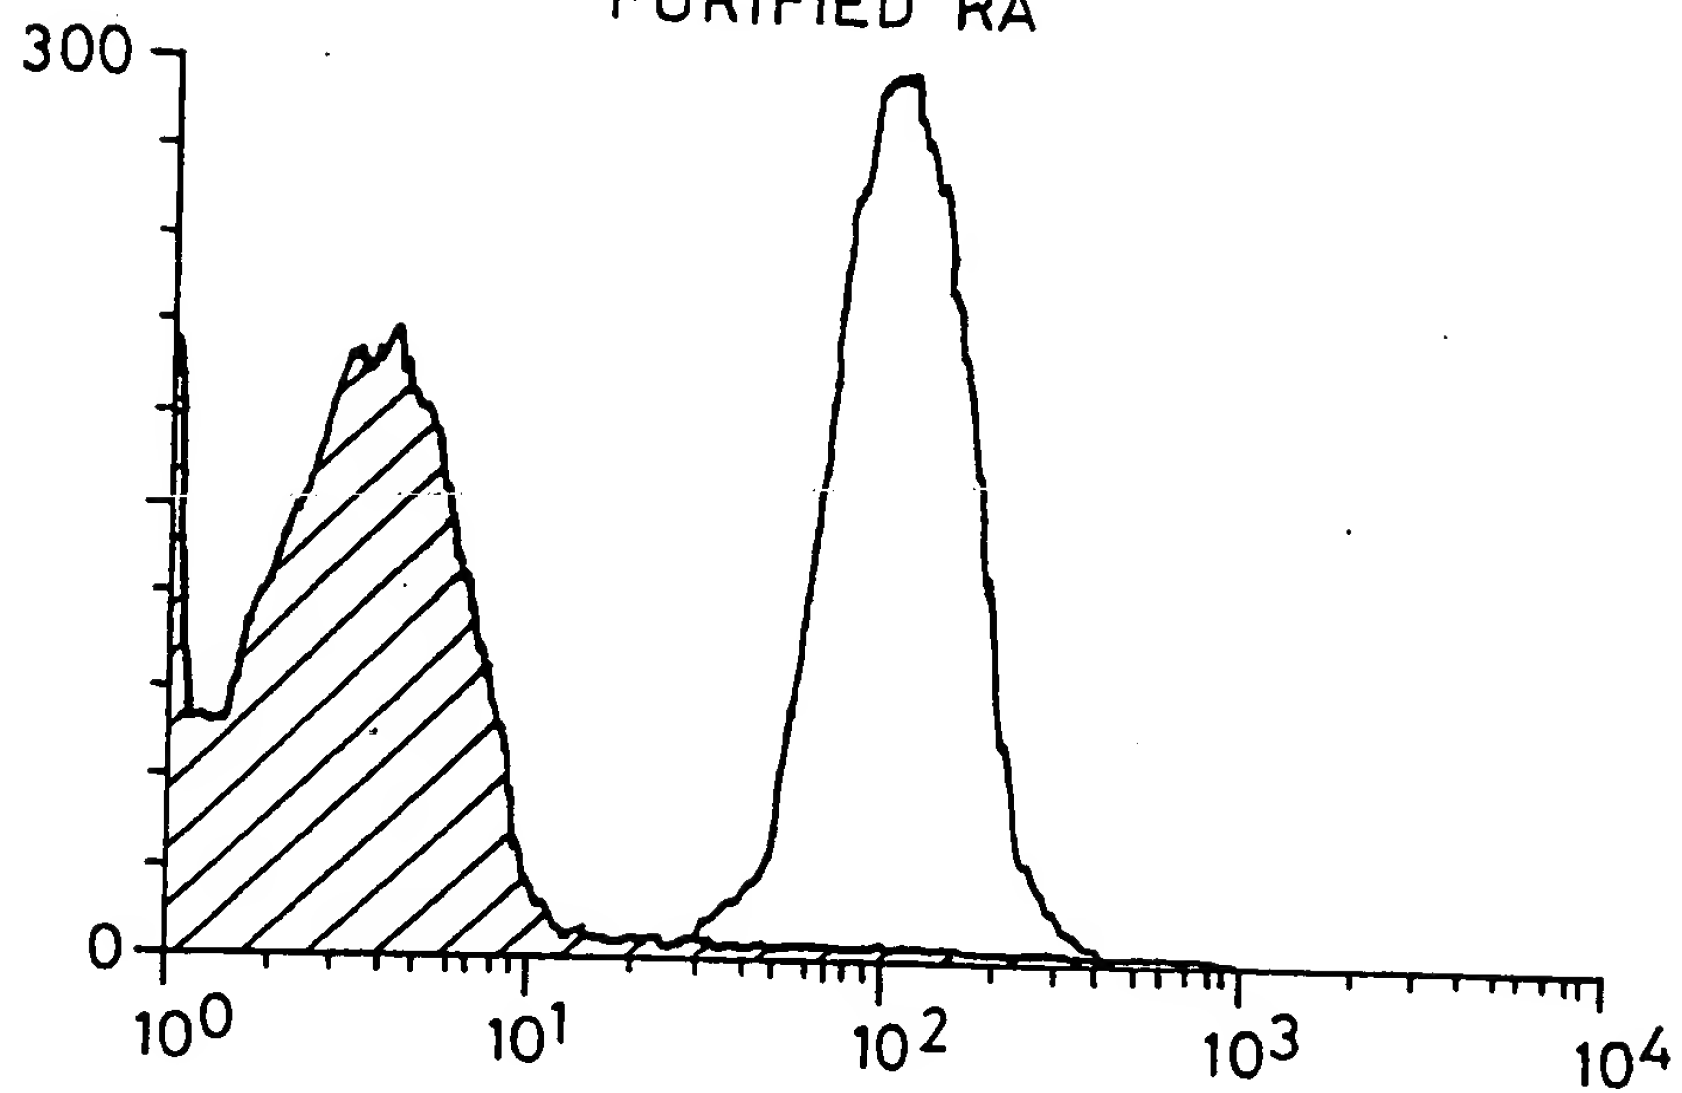


FIG. 3(B)

PURIFIED RO

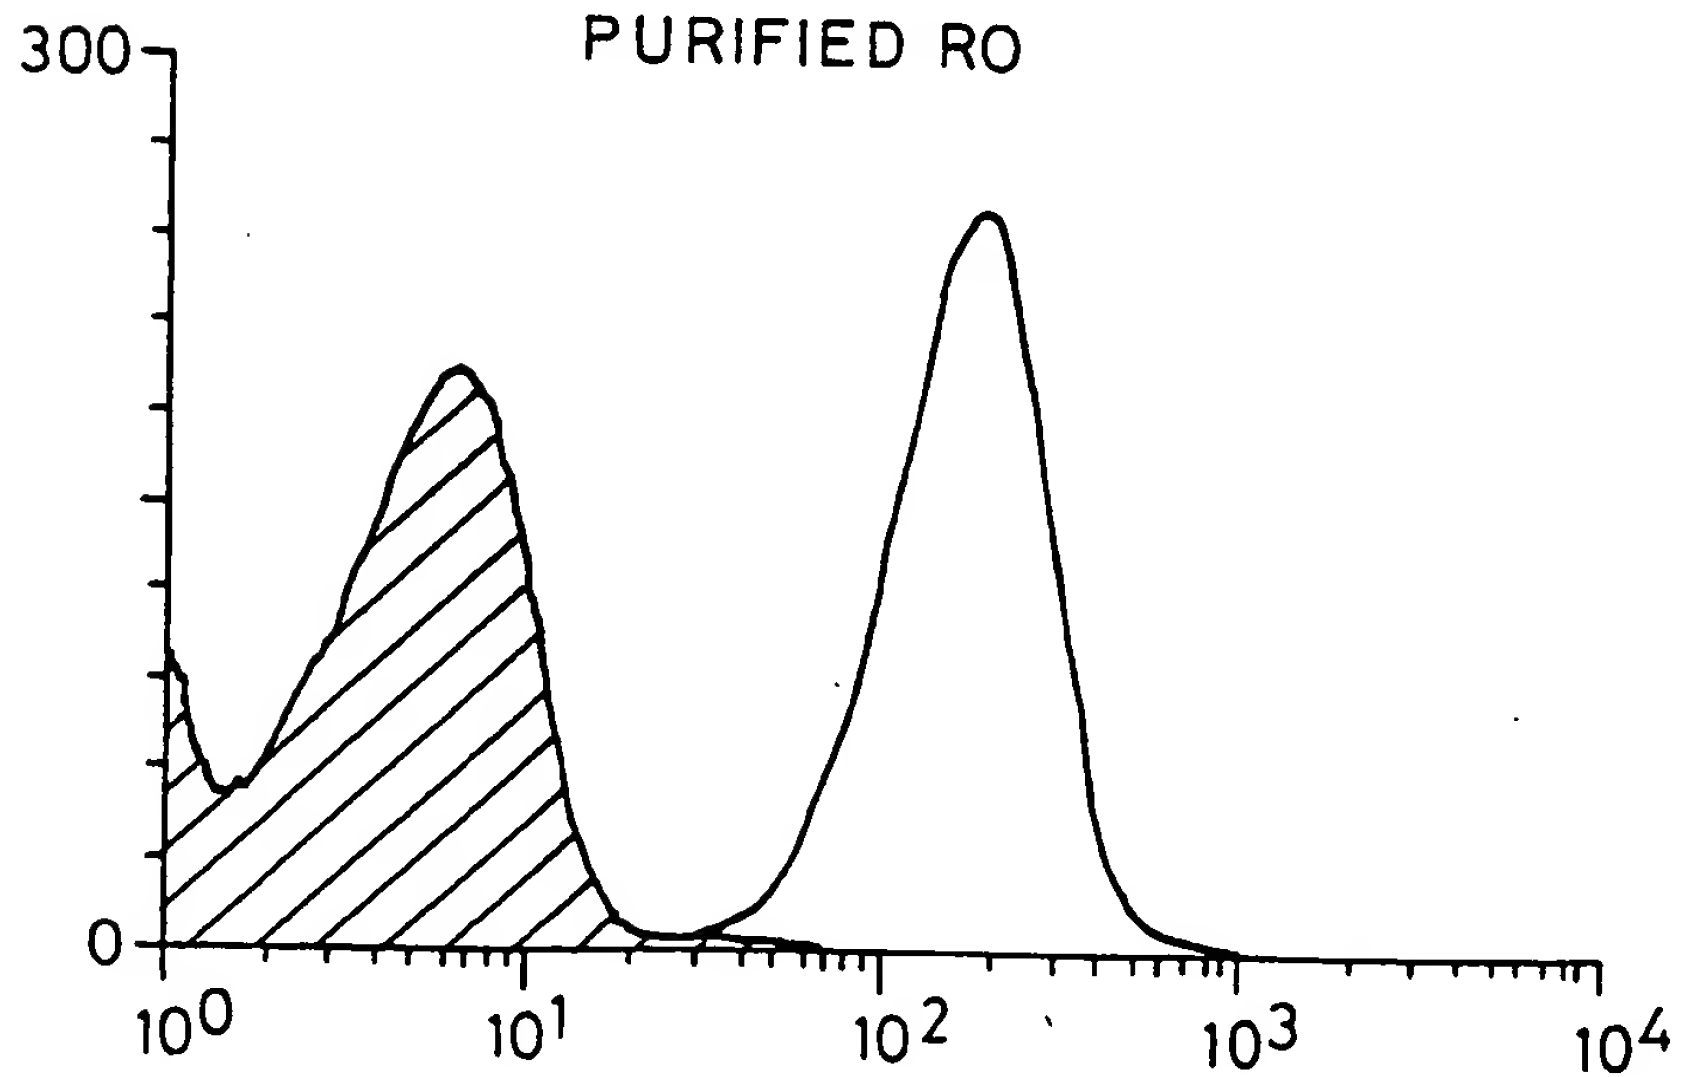

7/14

FIG. 3(C)

CORD BLOOD PURIF. RA


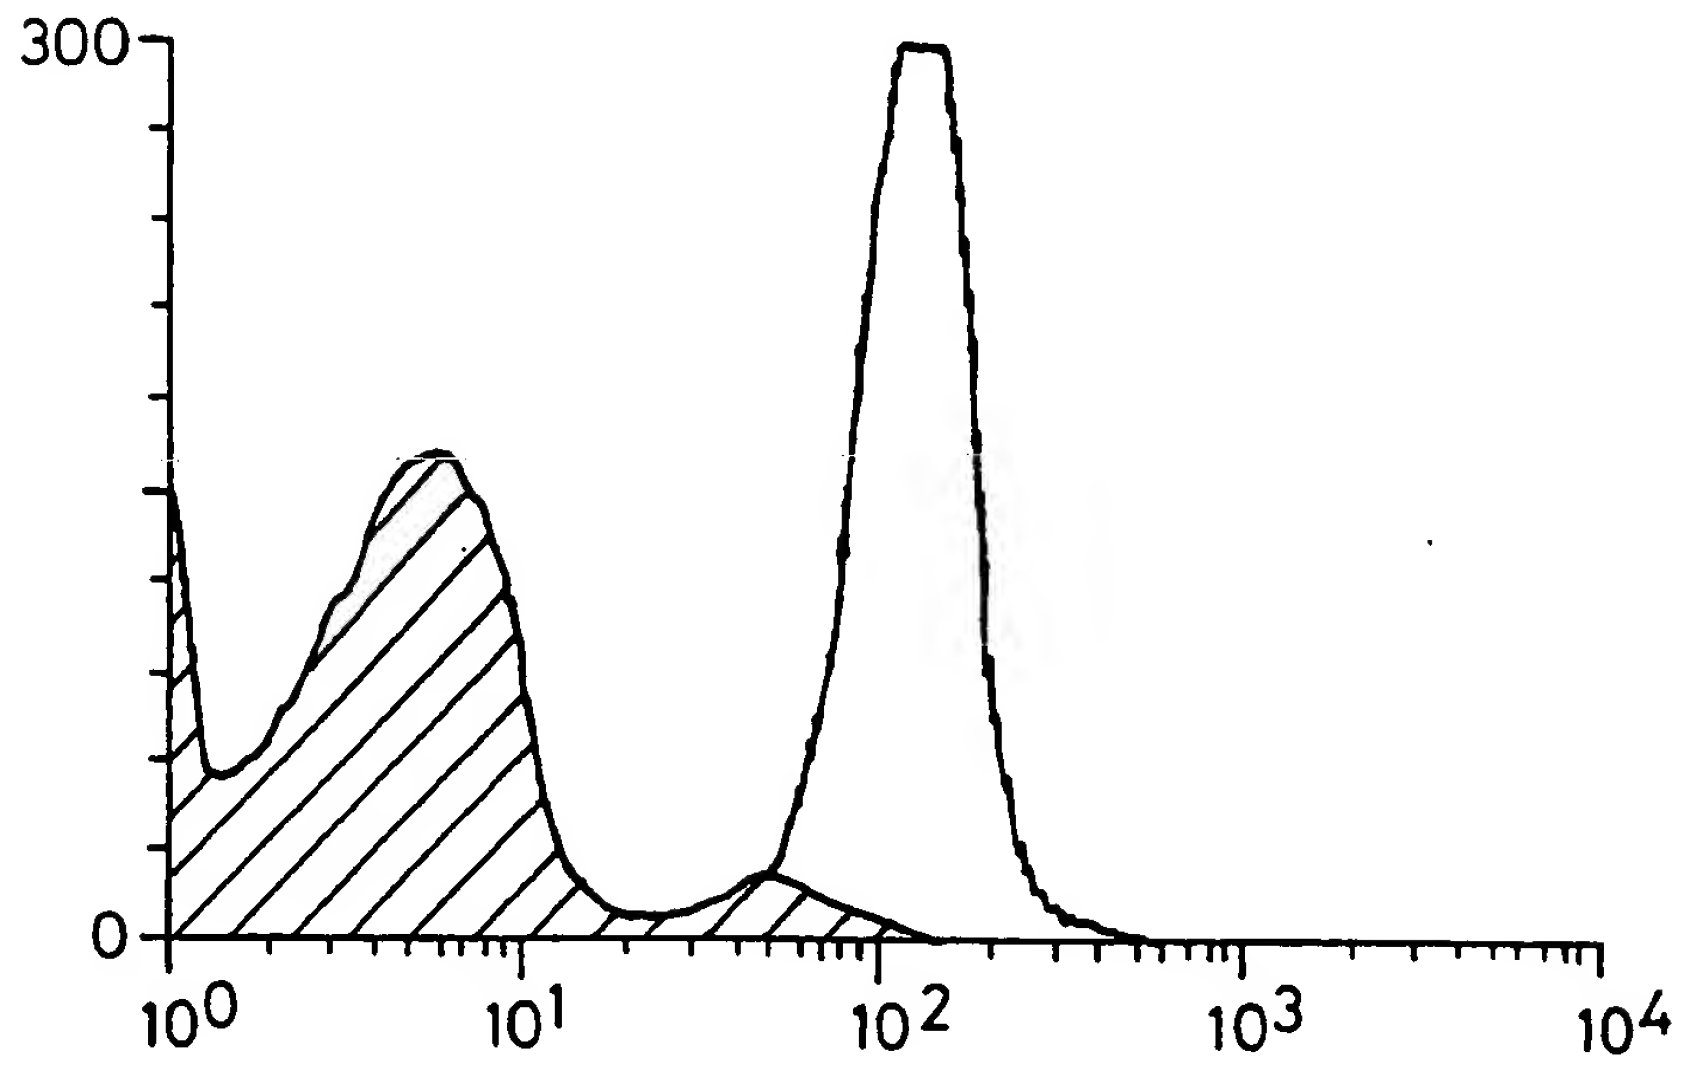


FIG. 3(D)

CORD BLOOD RA PHA STIM.



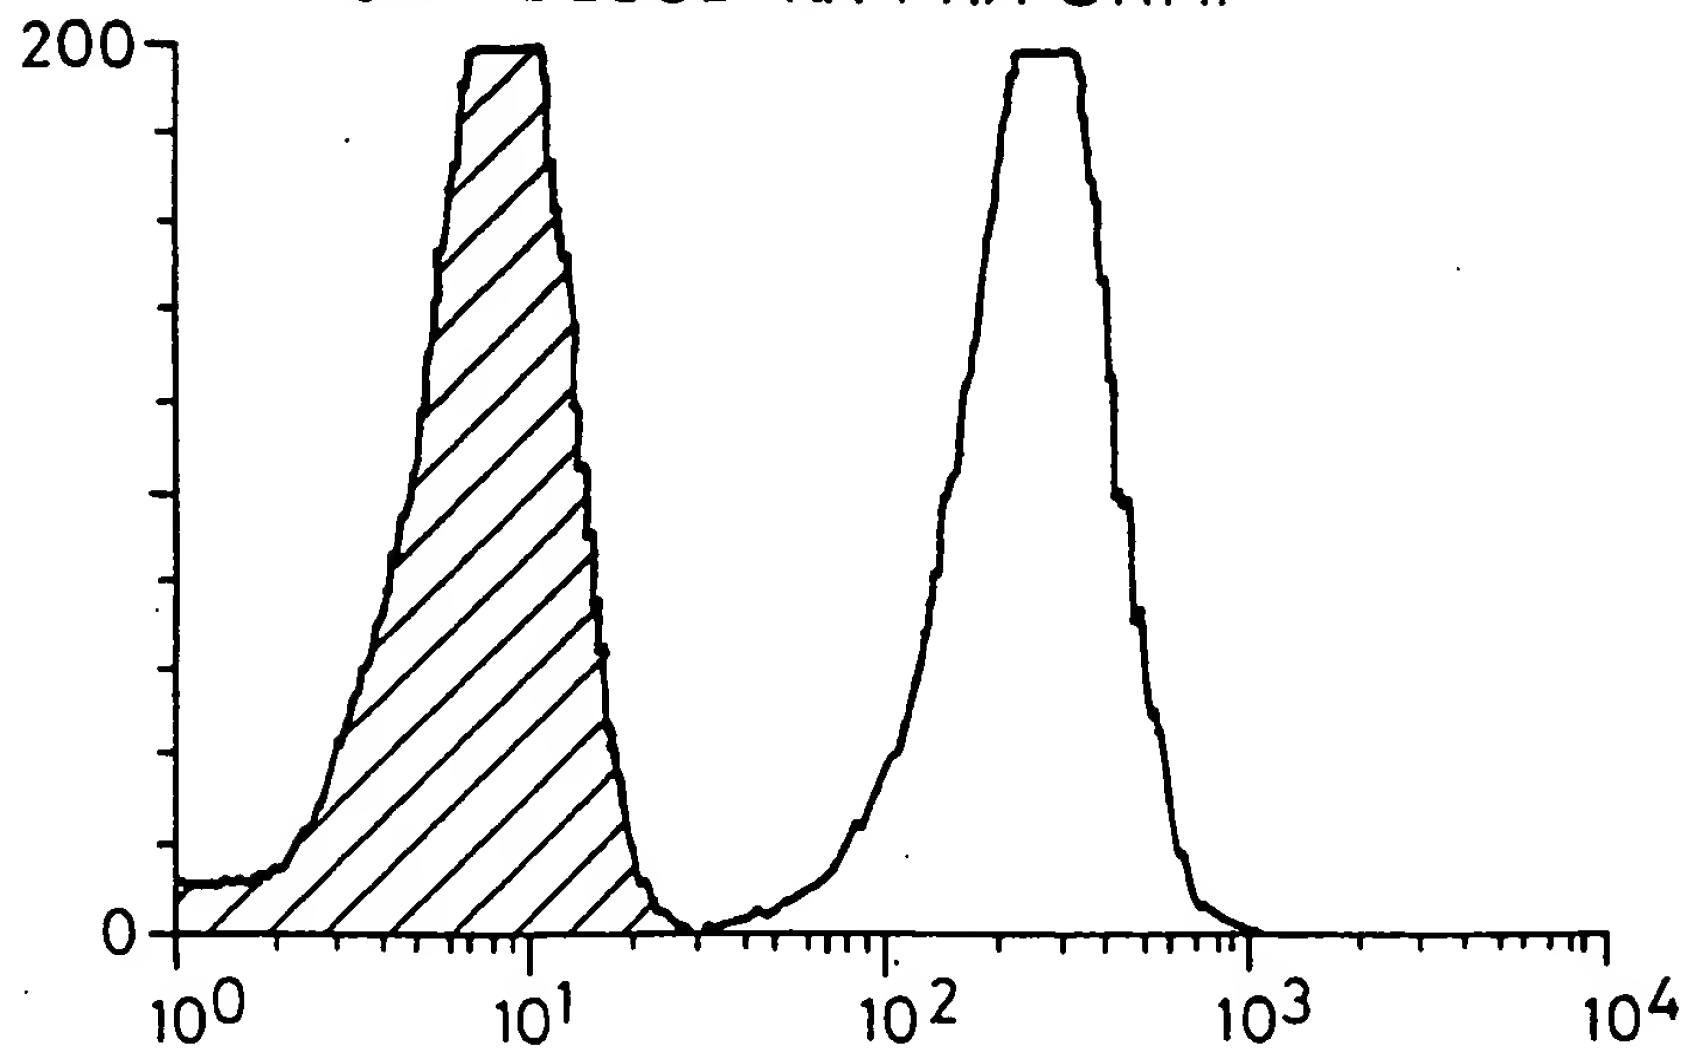

8/14

FIG. 3(E)

KC3 TCC


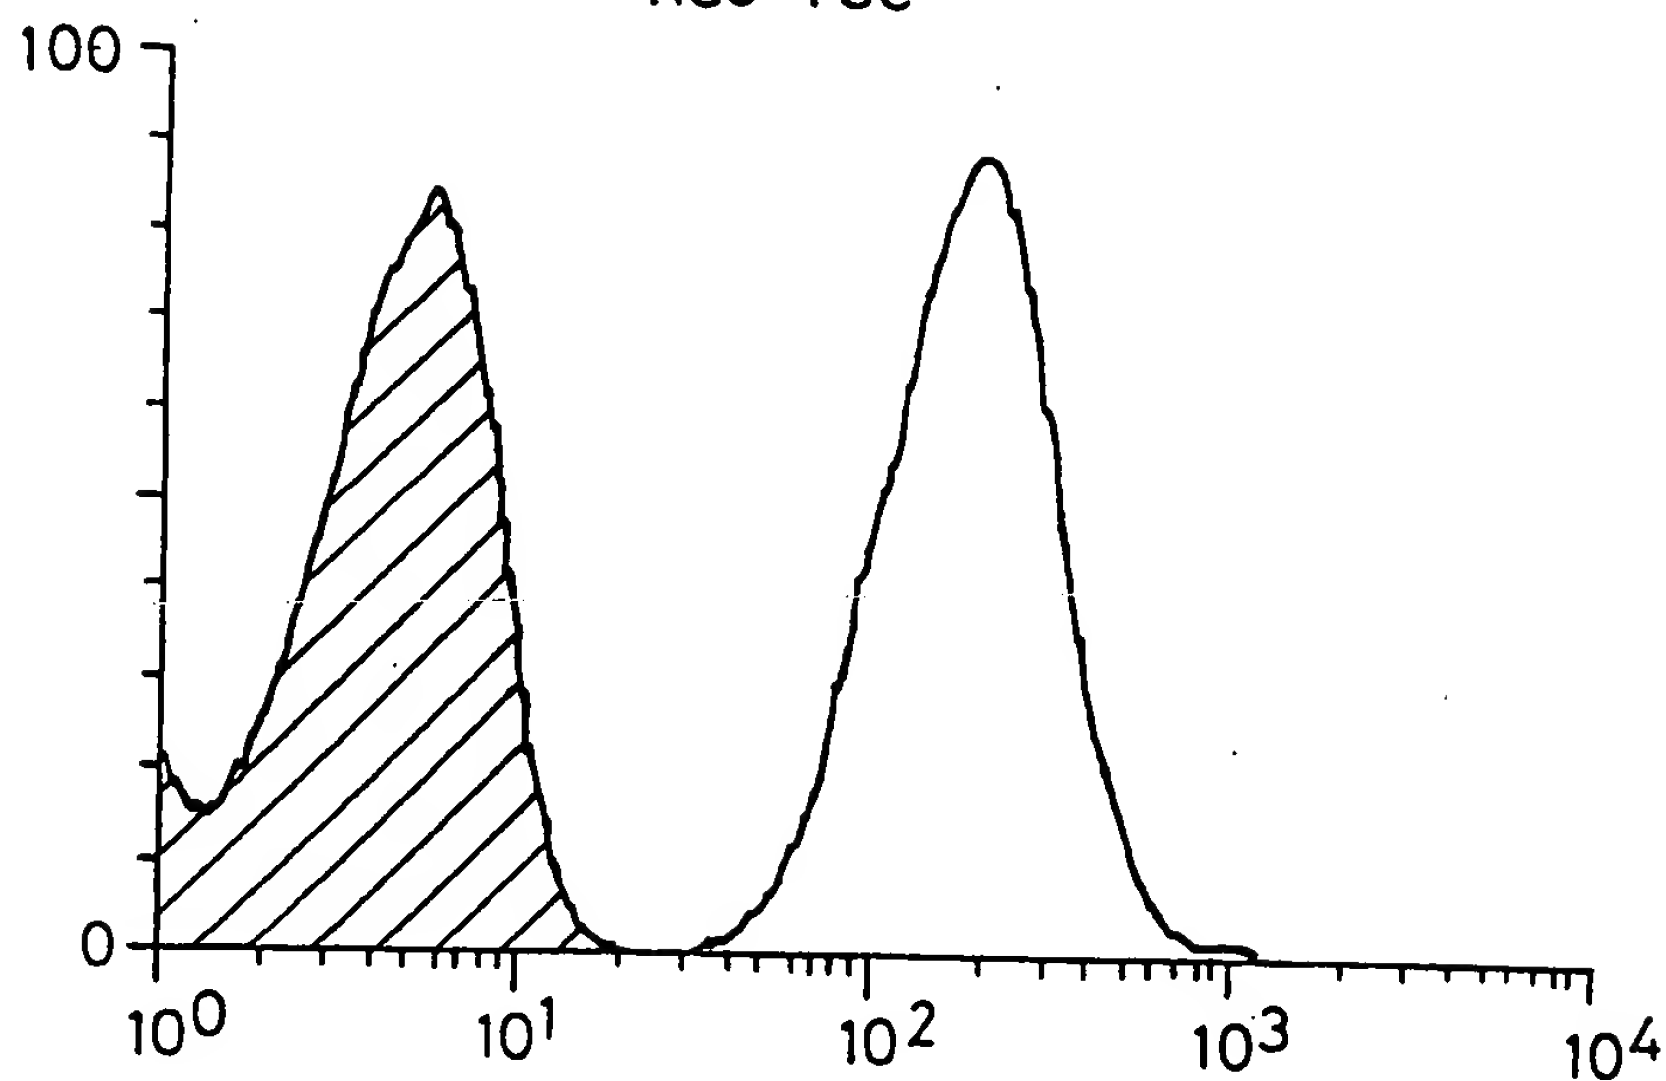



FIG. 3(F)

SAG S9 TCC

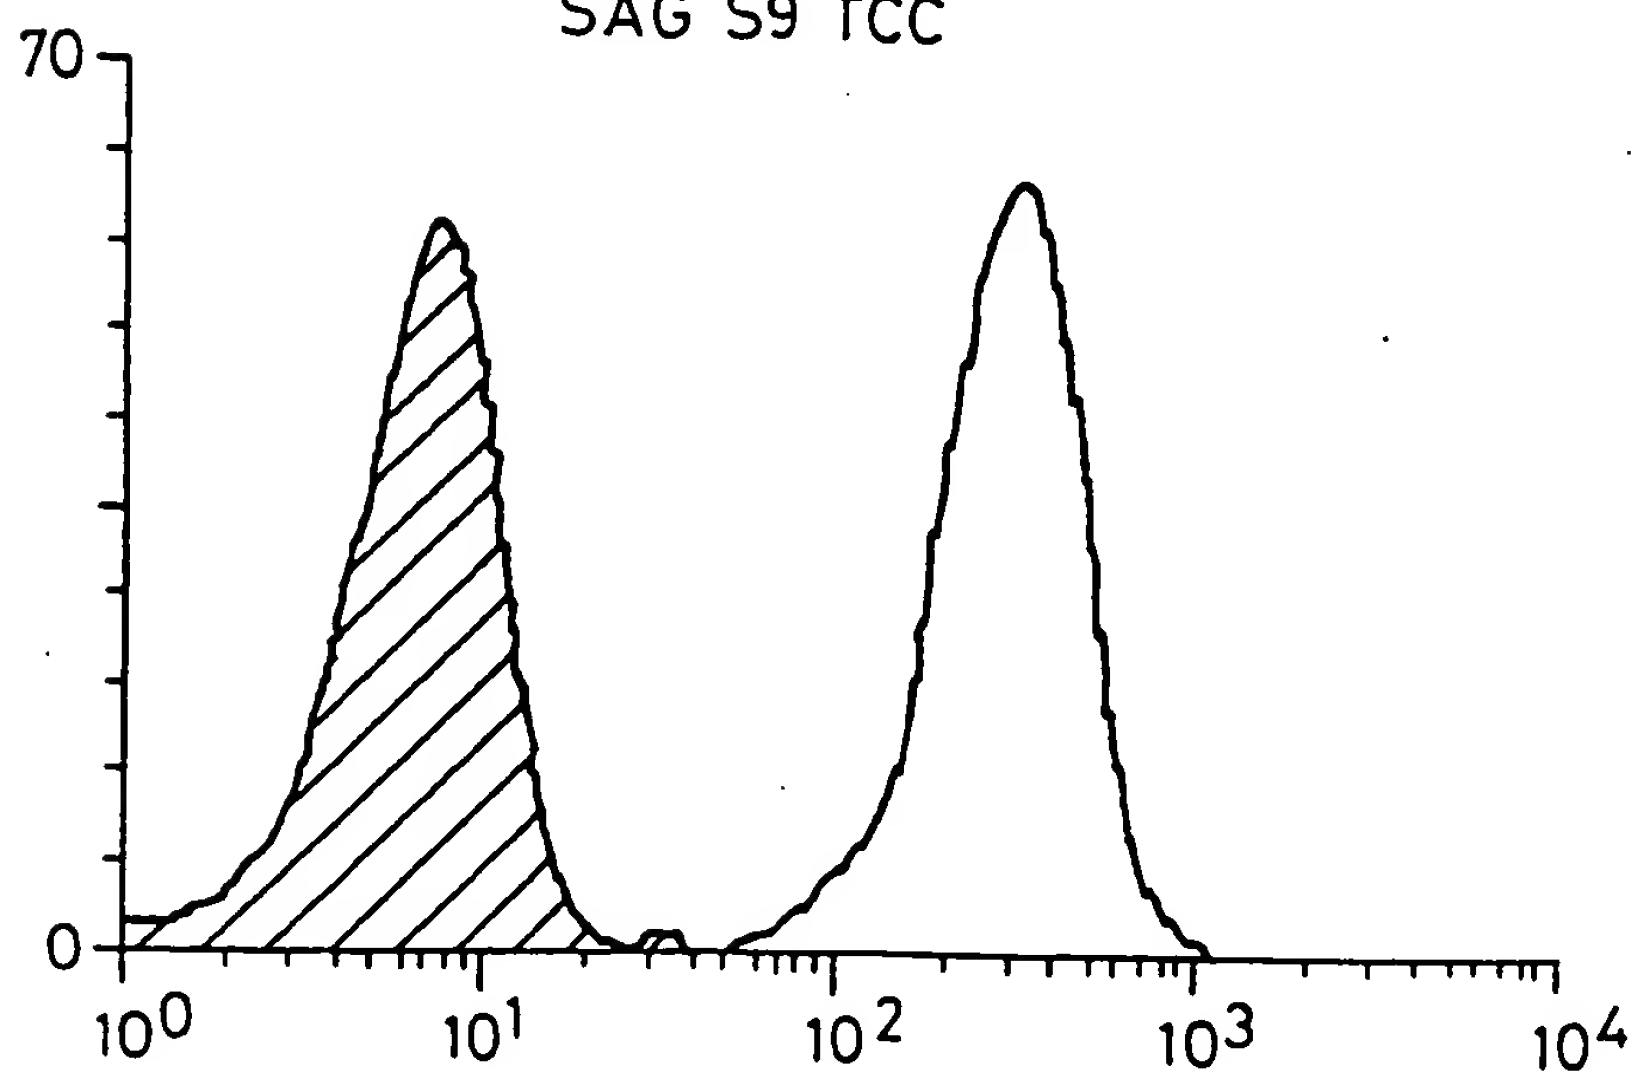

9/14

E2 CHO (CONF.)

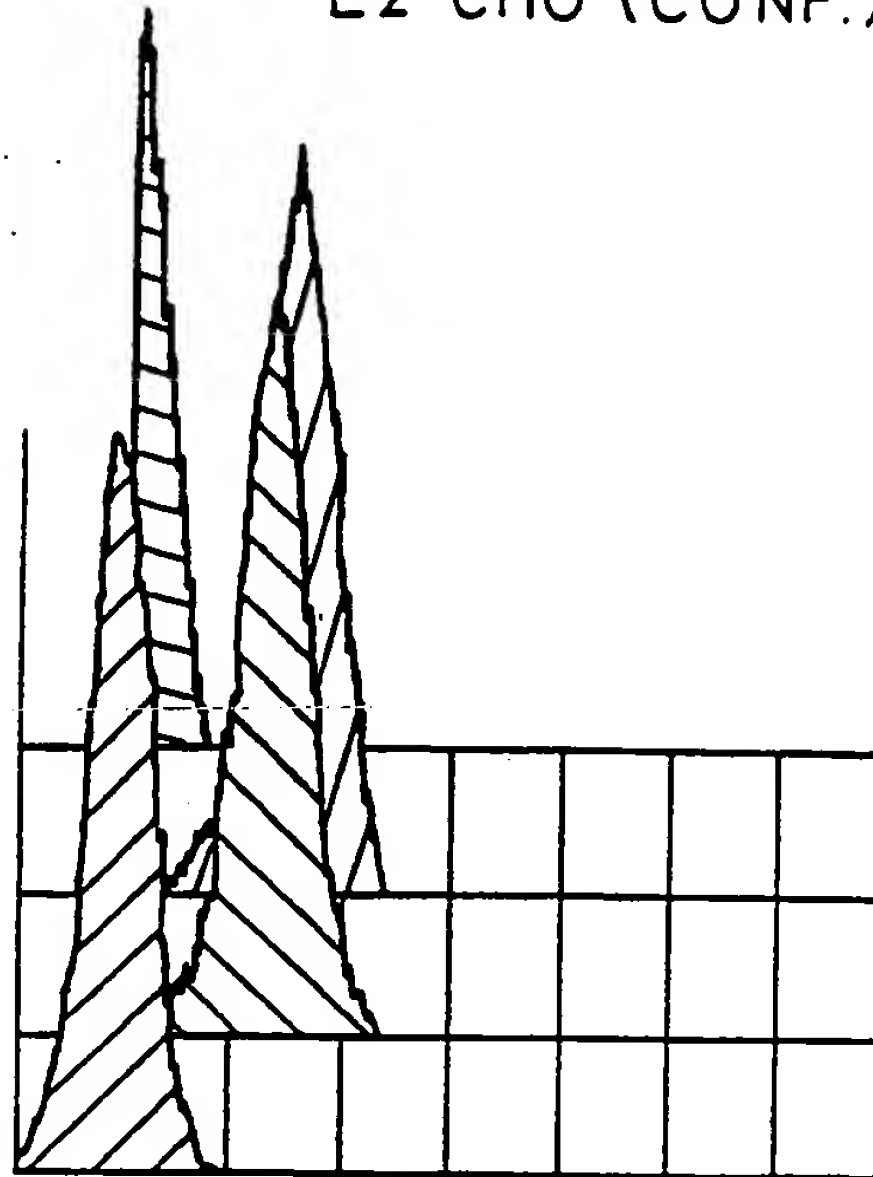

500 MMB-MERC.


BOILED (3 MIN.)

POSITIVE/CONTROL

NEGATIVE/CONTROL

FIG. 4

E2 CHO (CONF.)

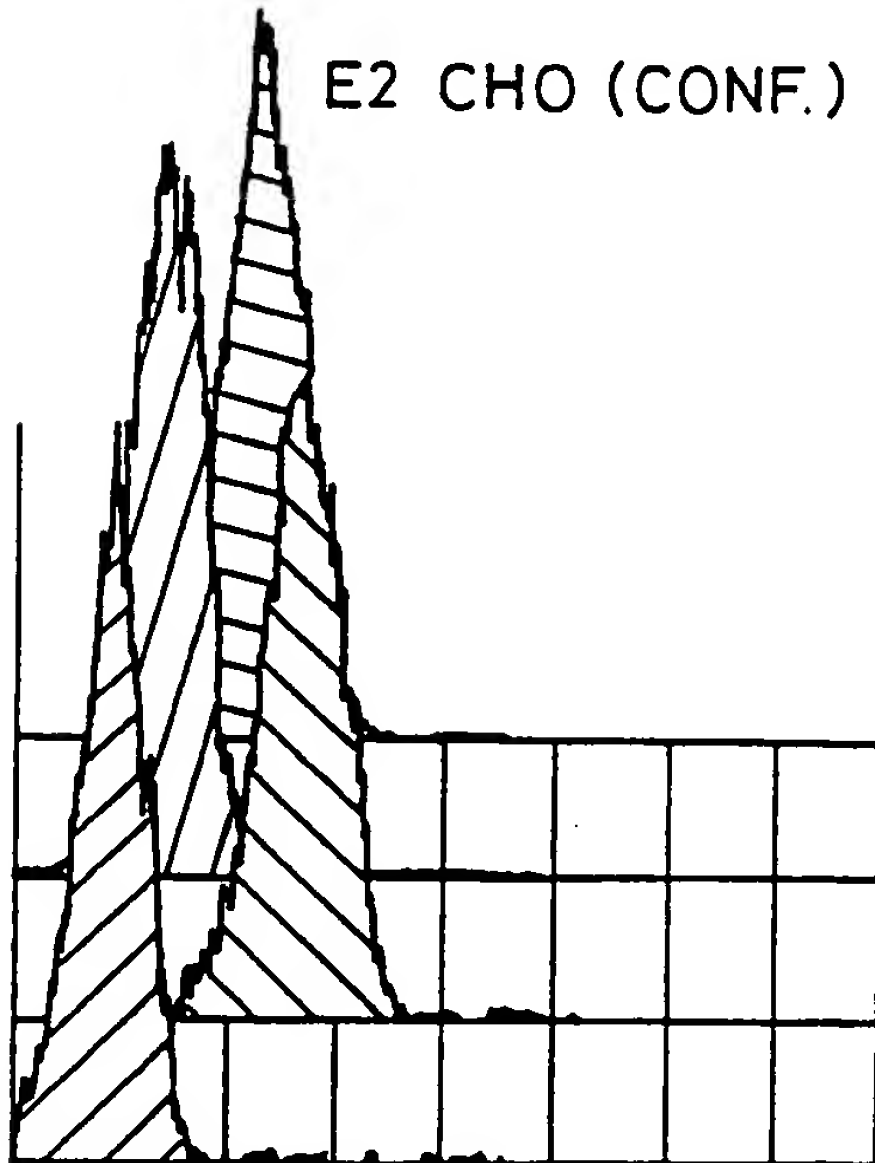

BOILED (10 MIN.)

0.2 U/ML ENDO H

POSITIVE/CONTROL

NEGATIVE CONTROL

FIG. 5

10/14

FIG. 6


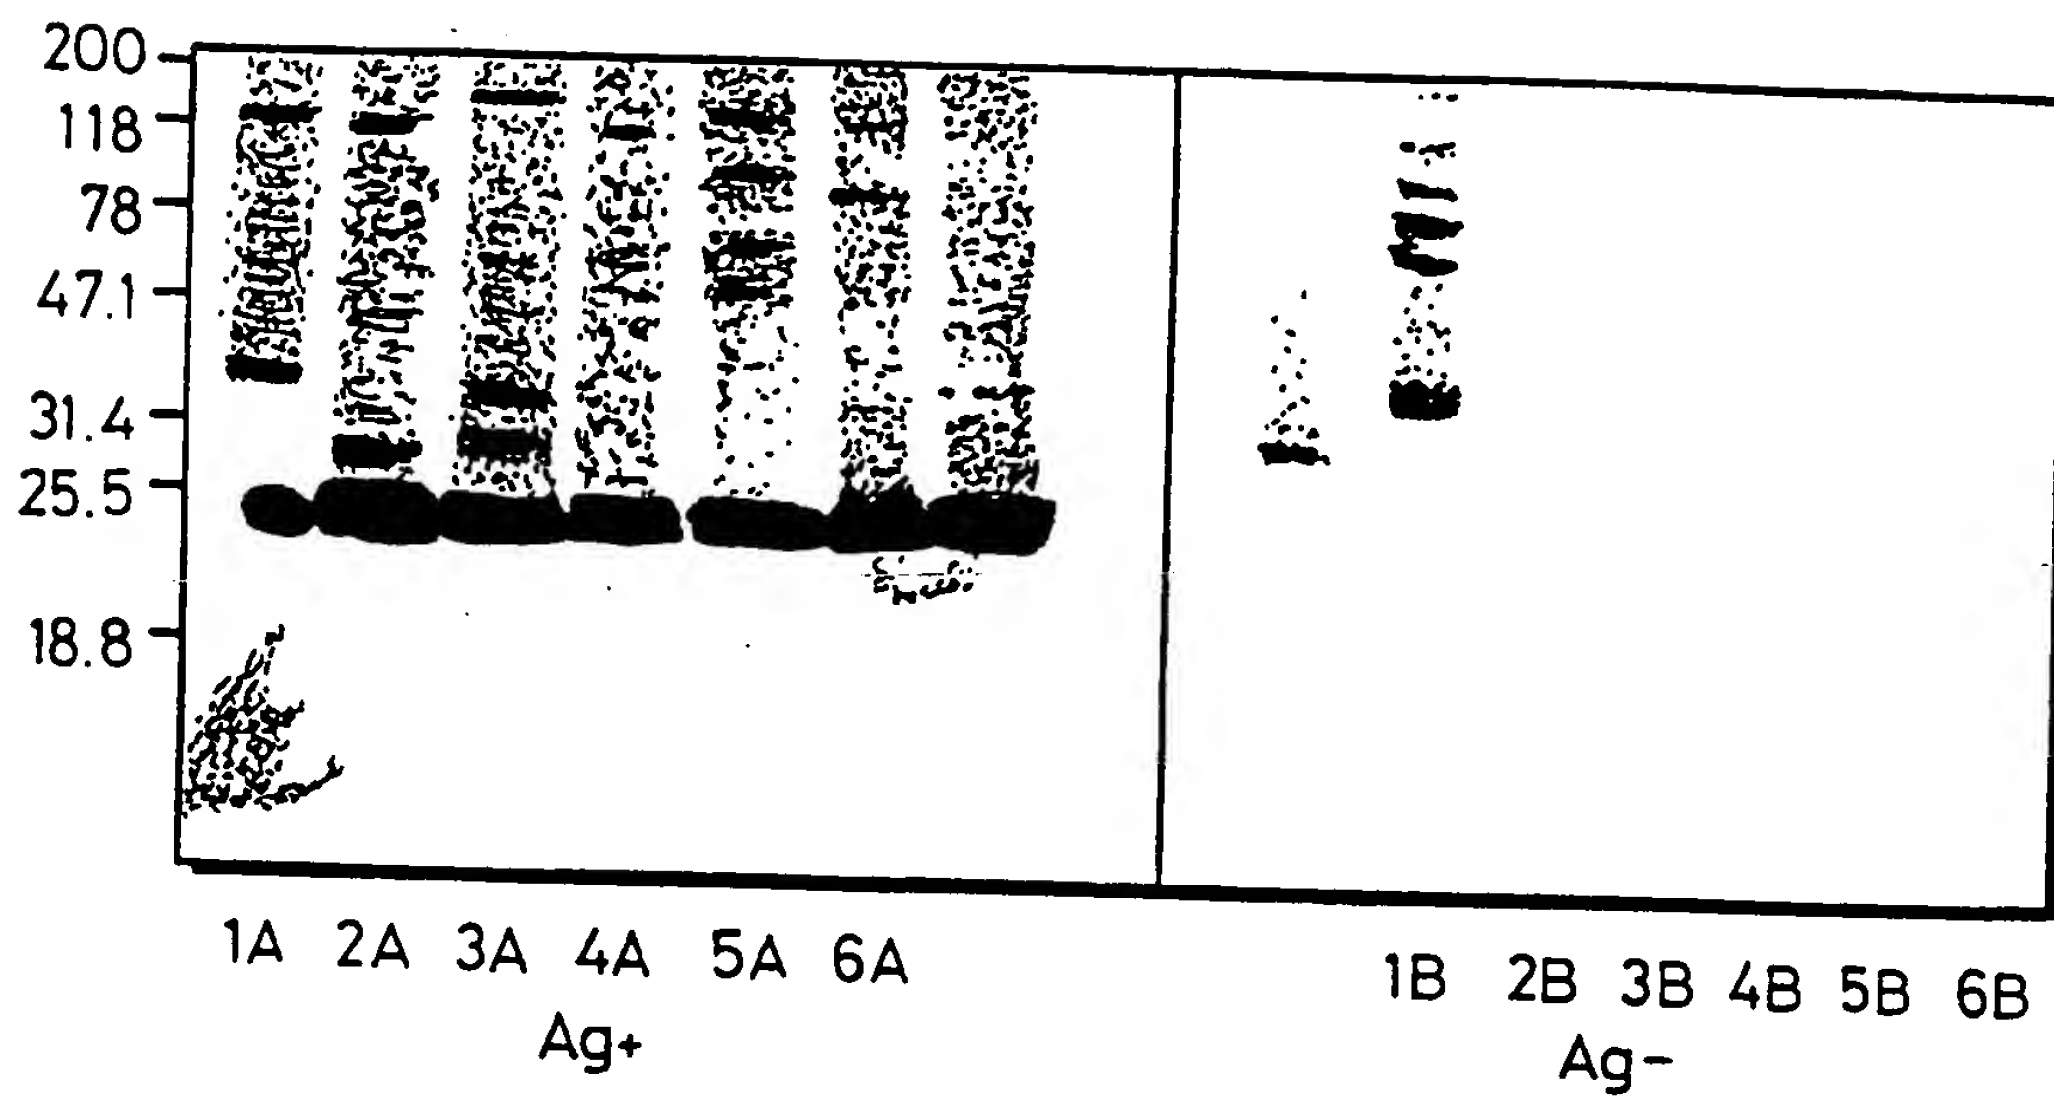


FIG. 7

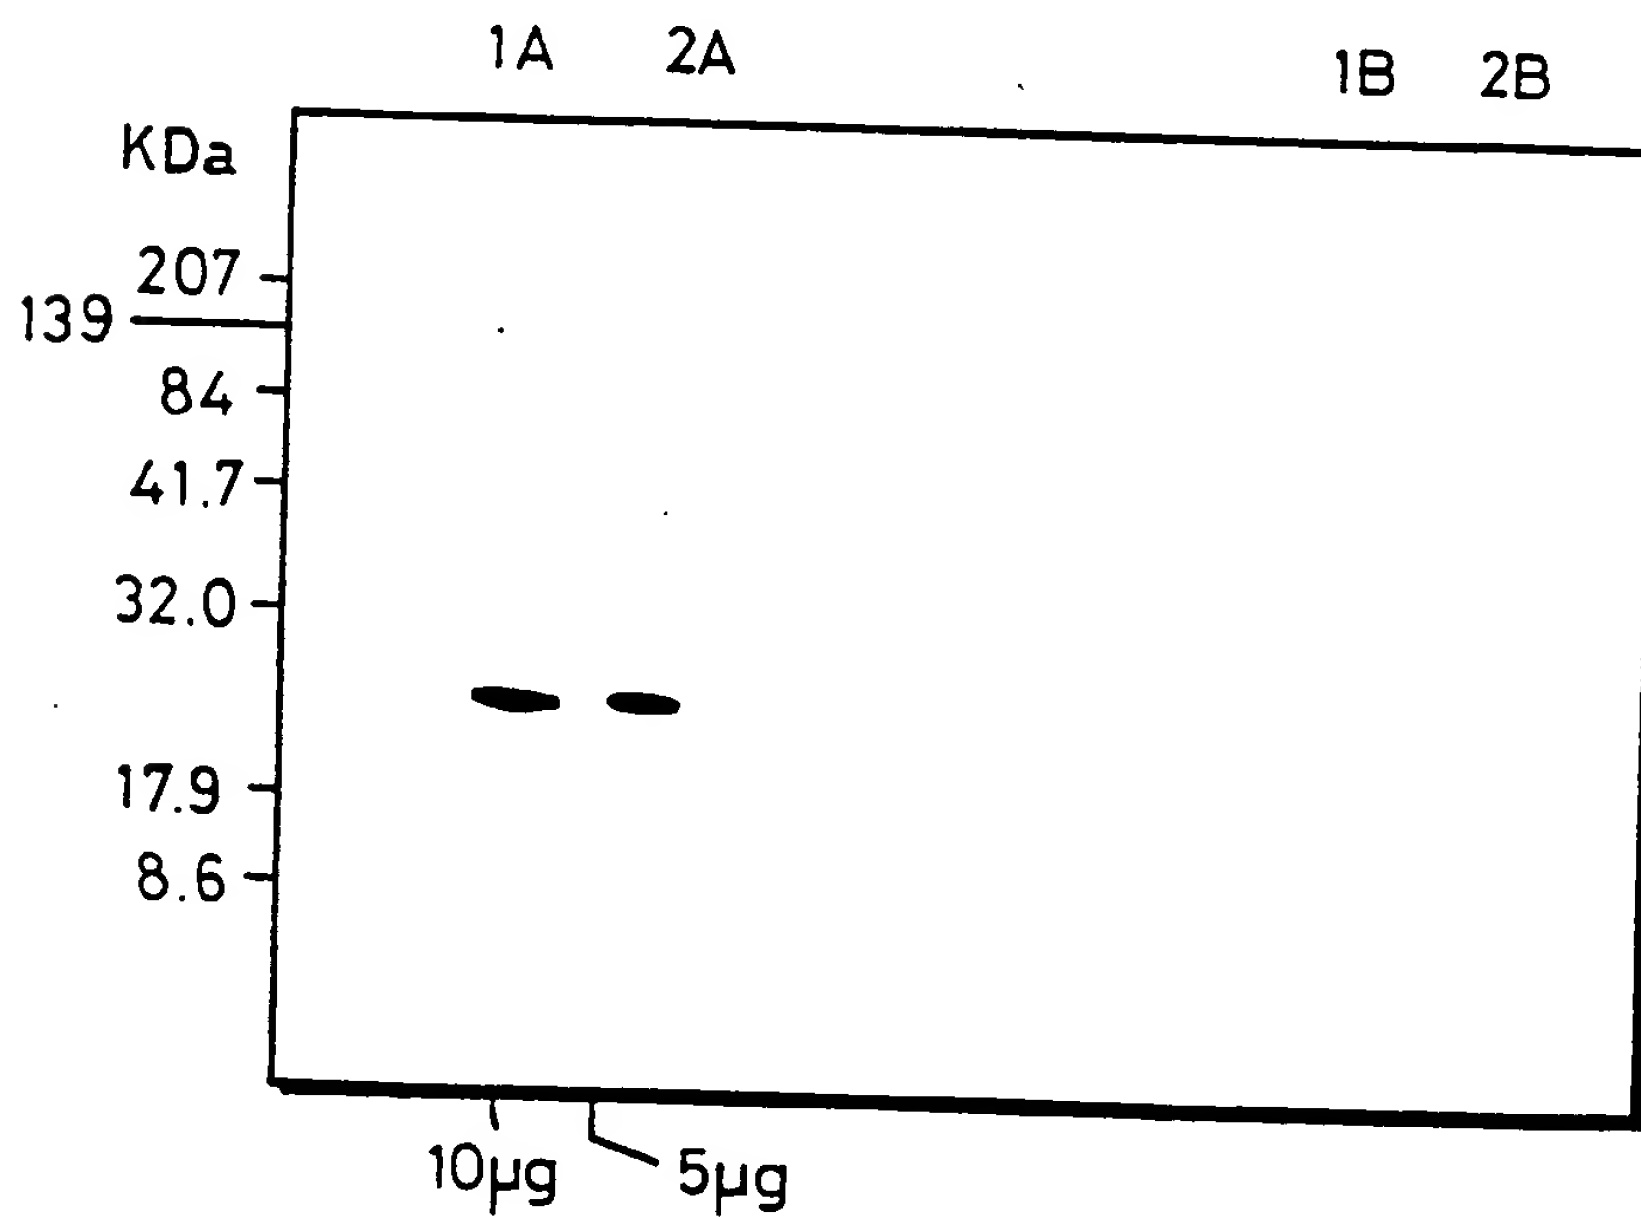

11/14

FIG. 8


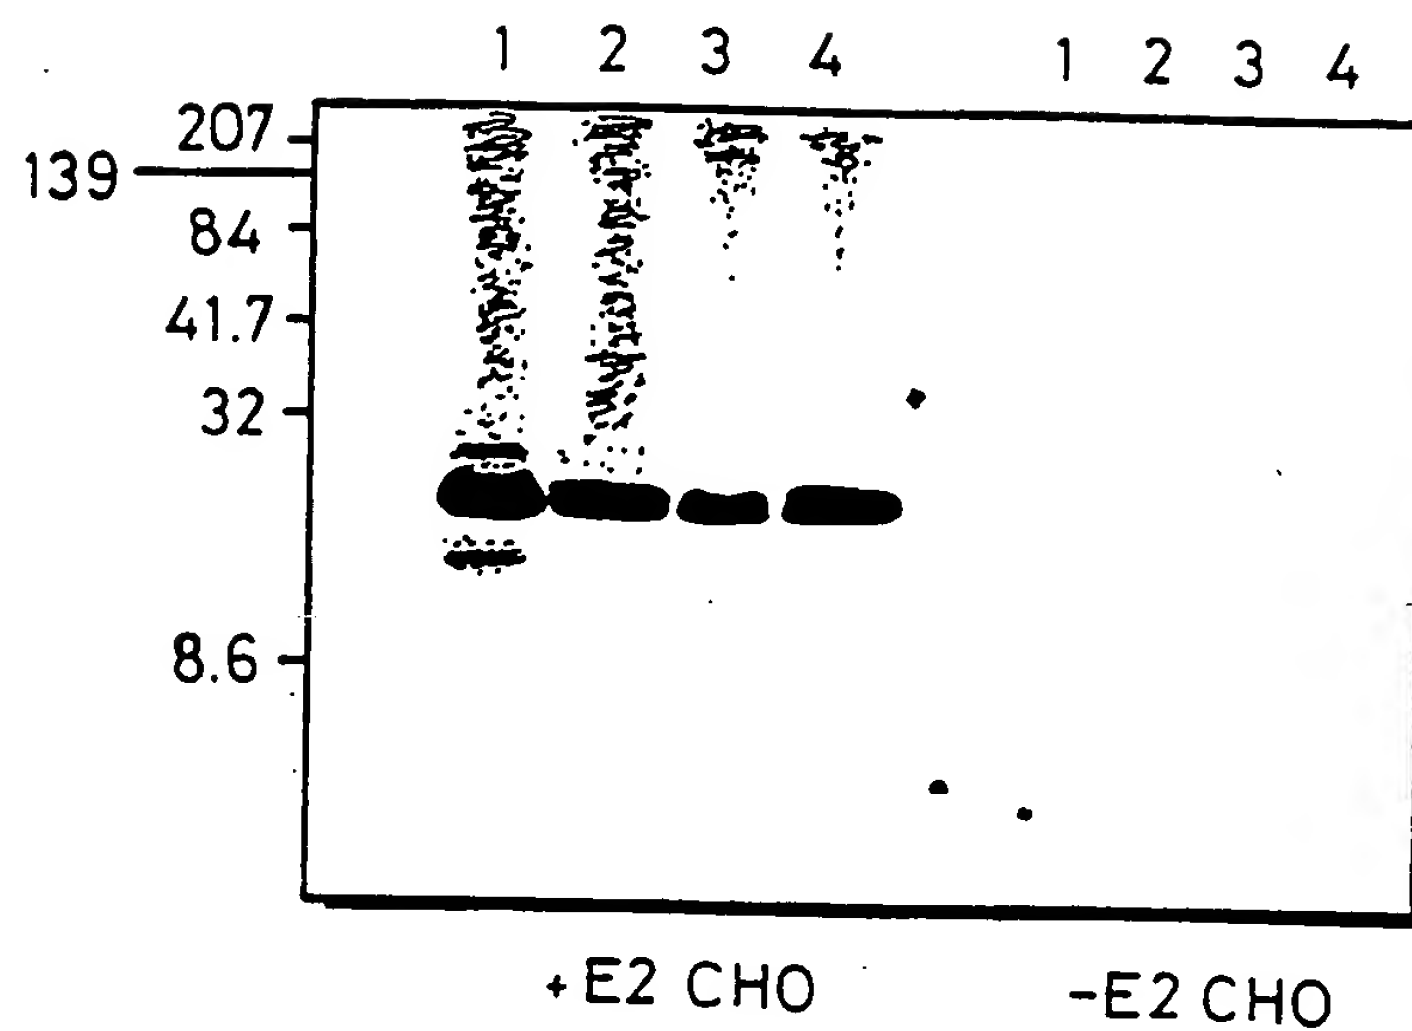


FIG. 9

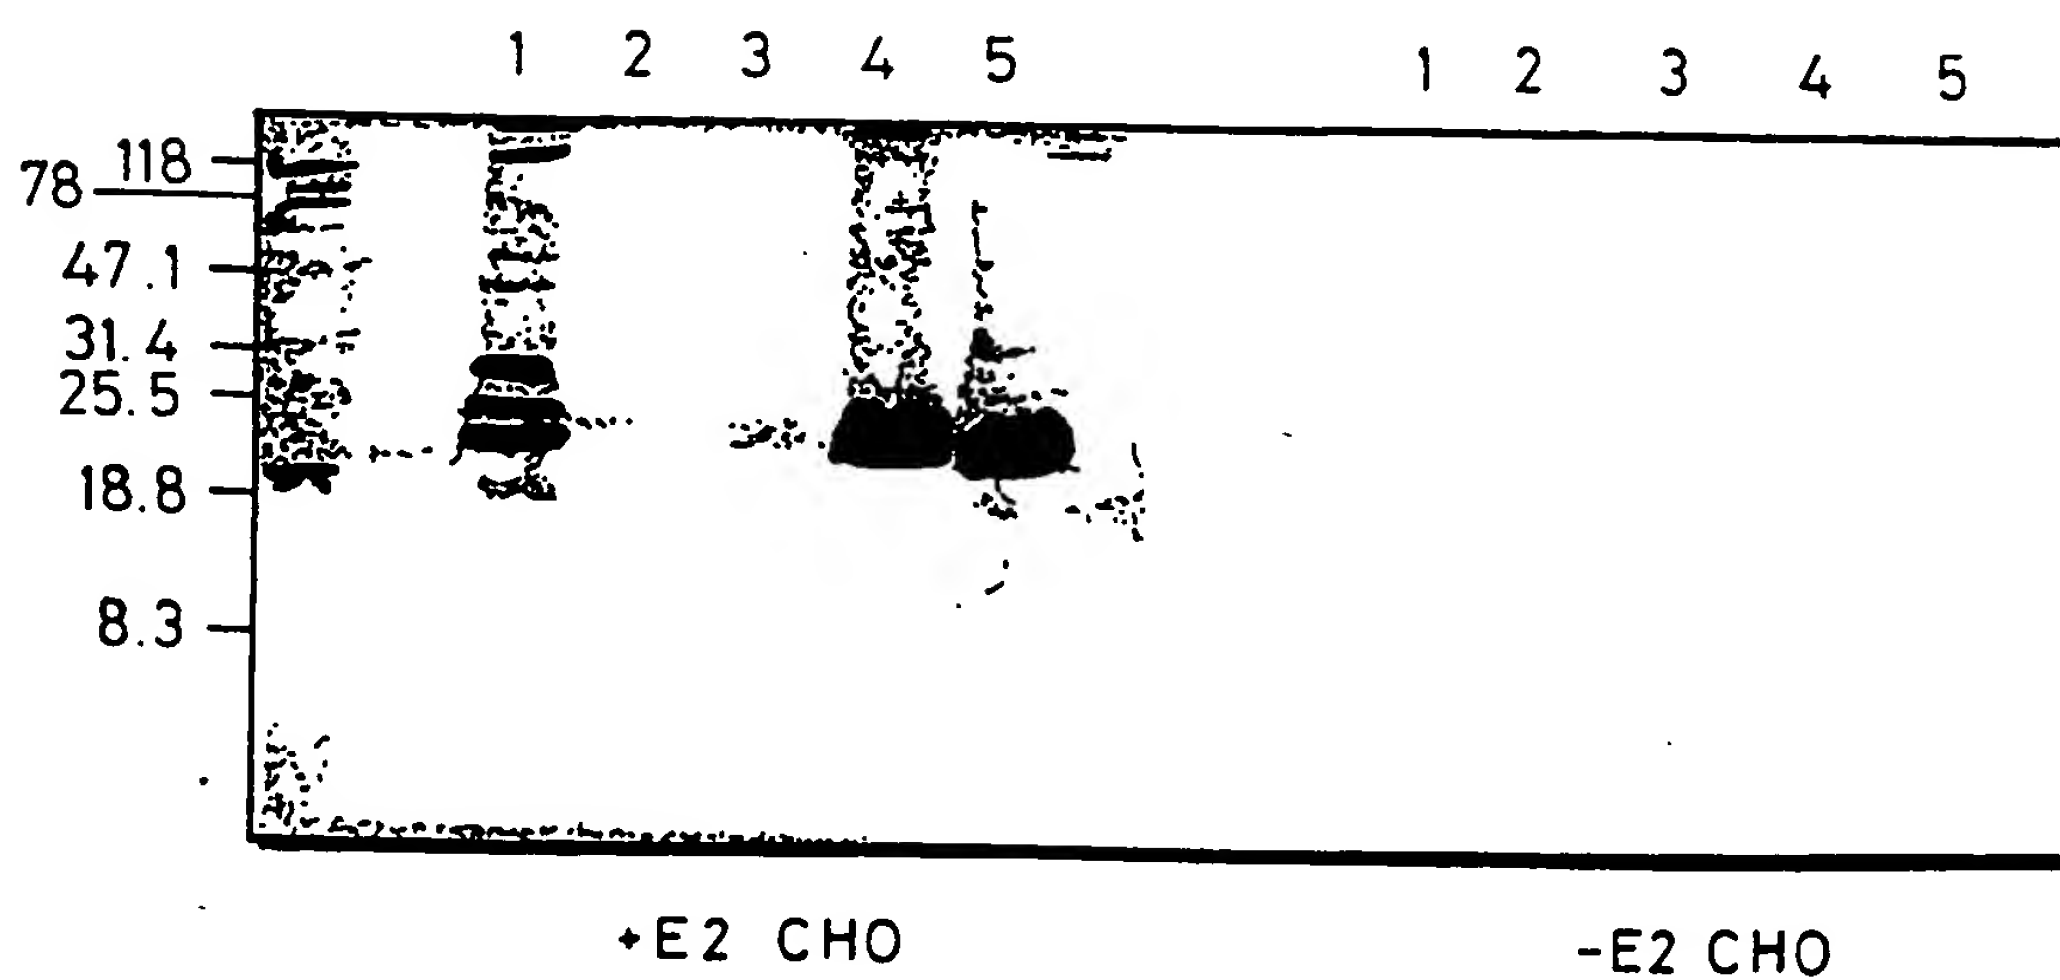

12/14

FIG. 10



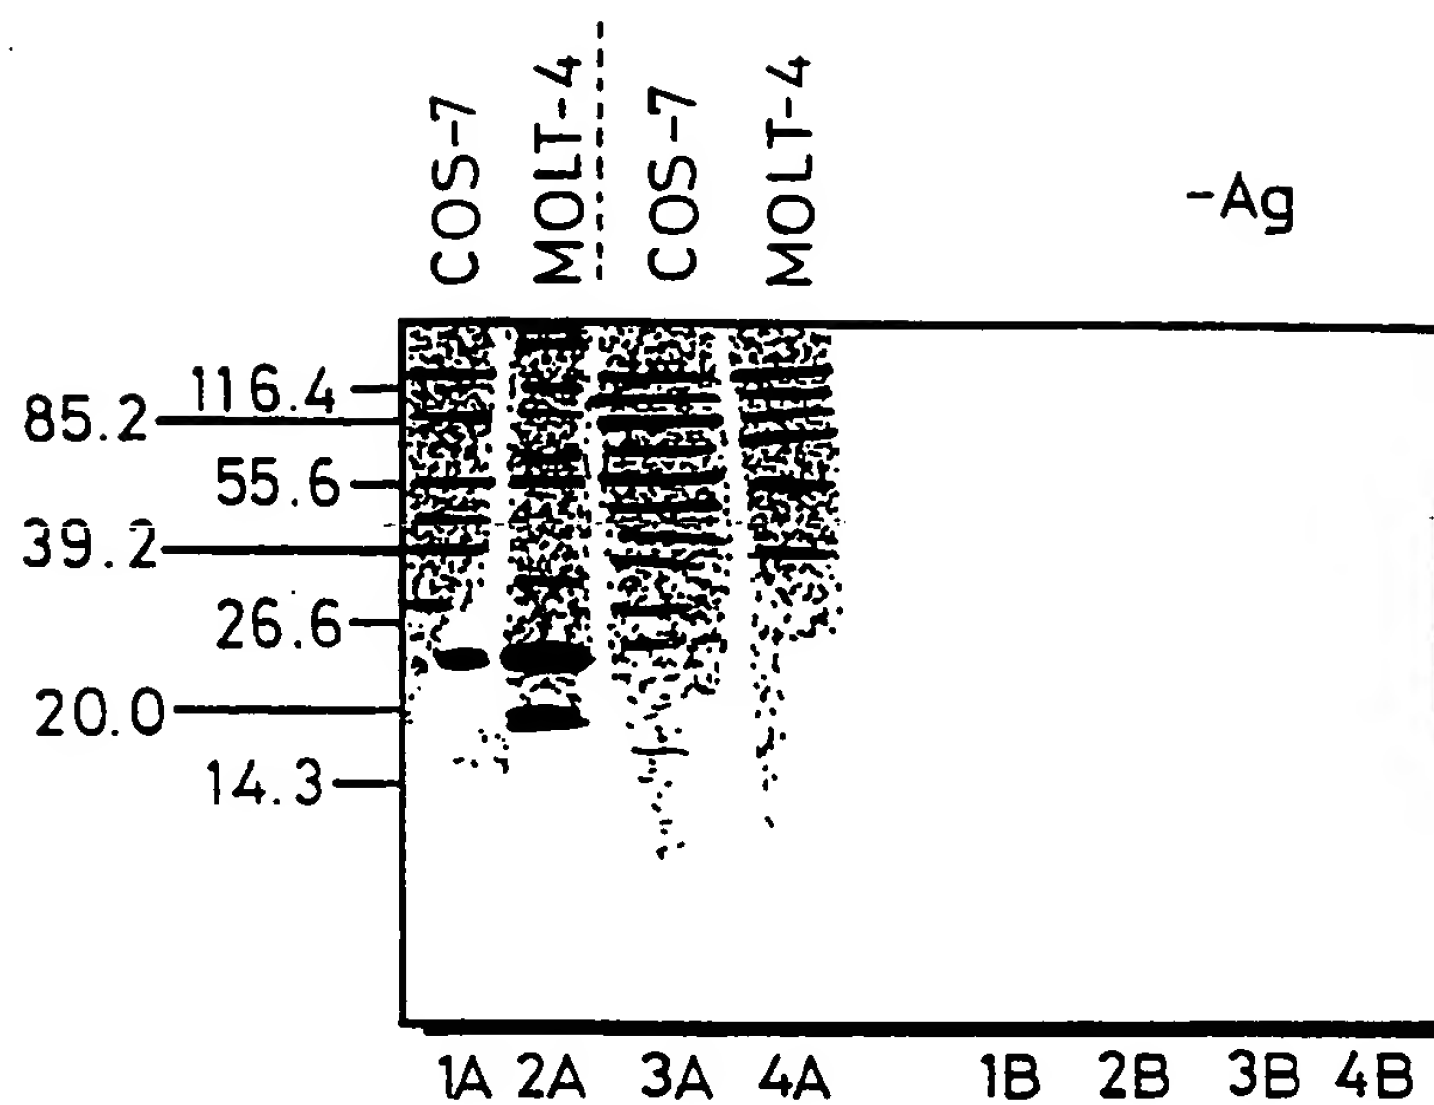


FIG. 11

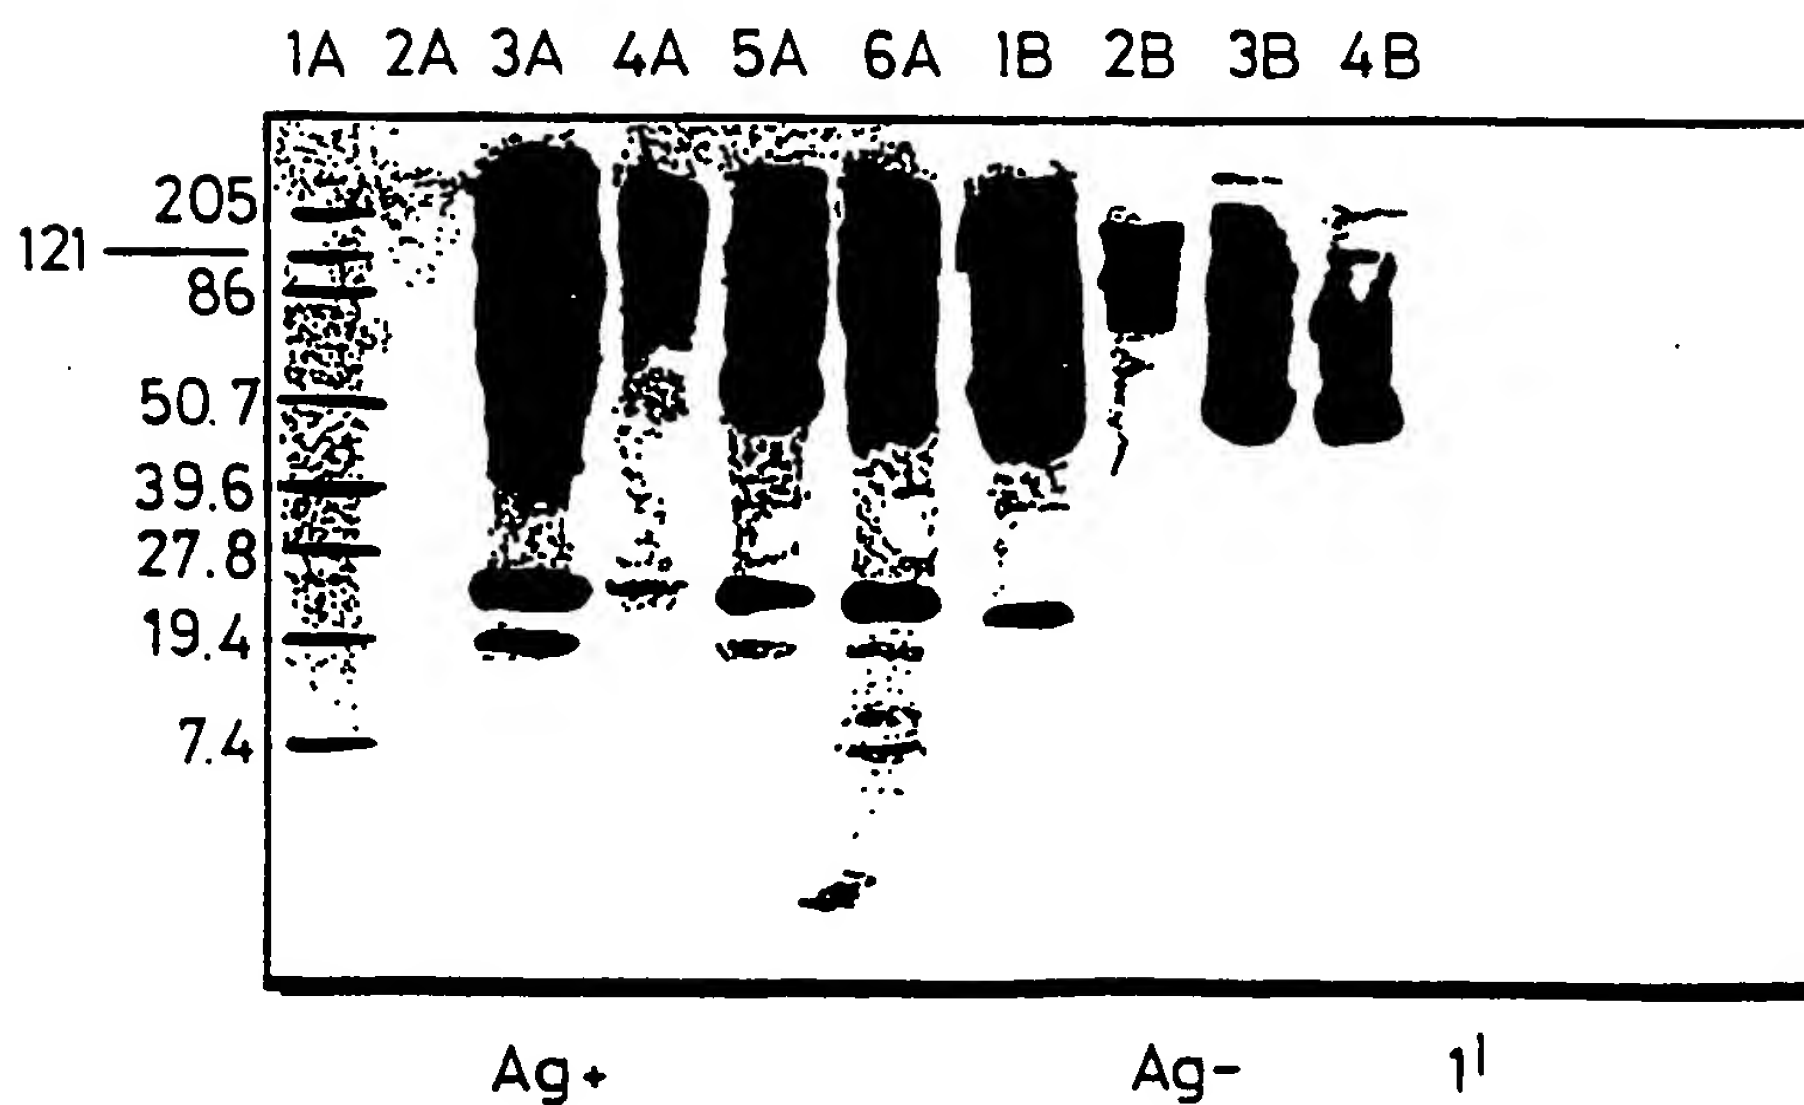

13/14

FIG. 12

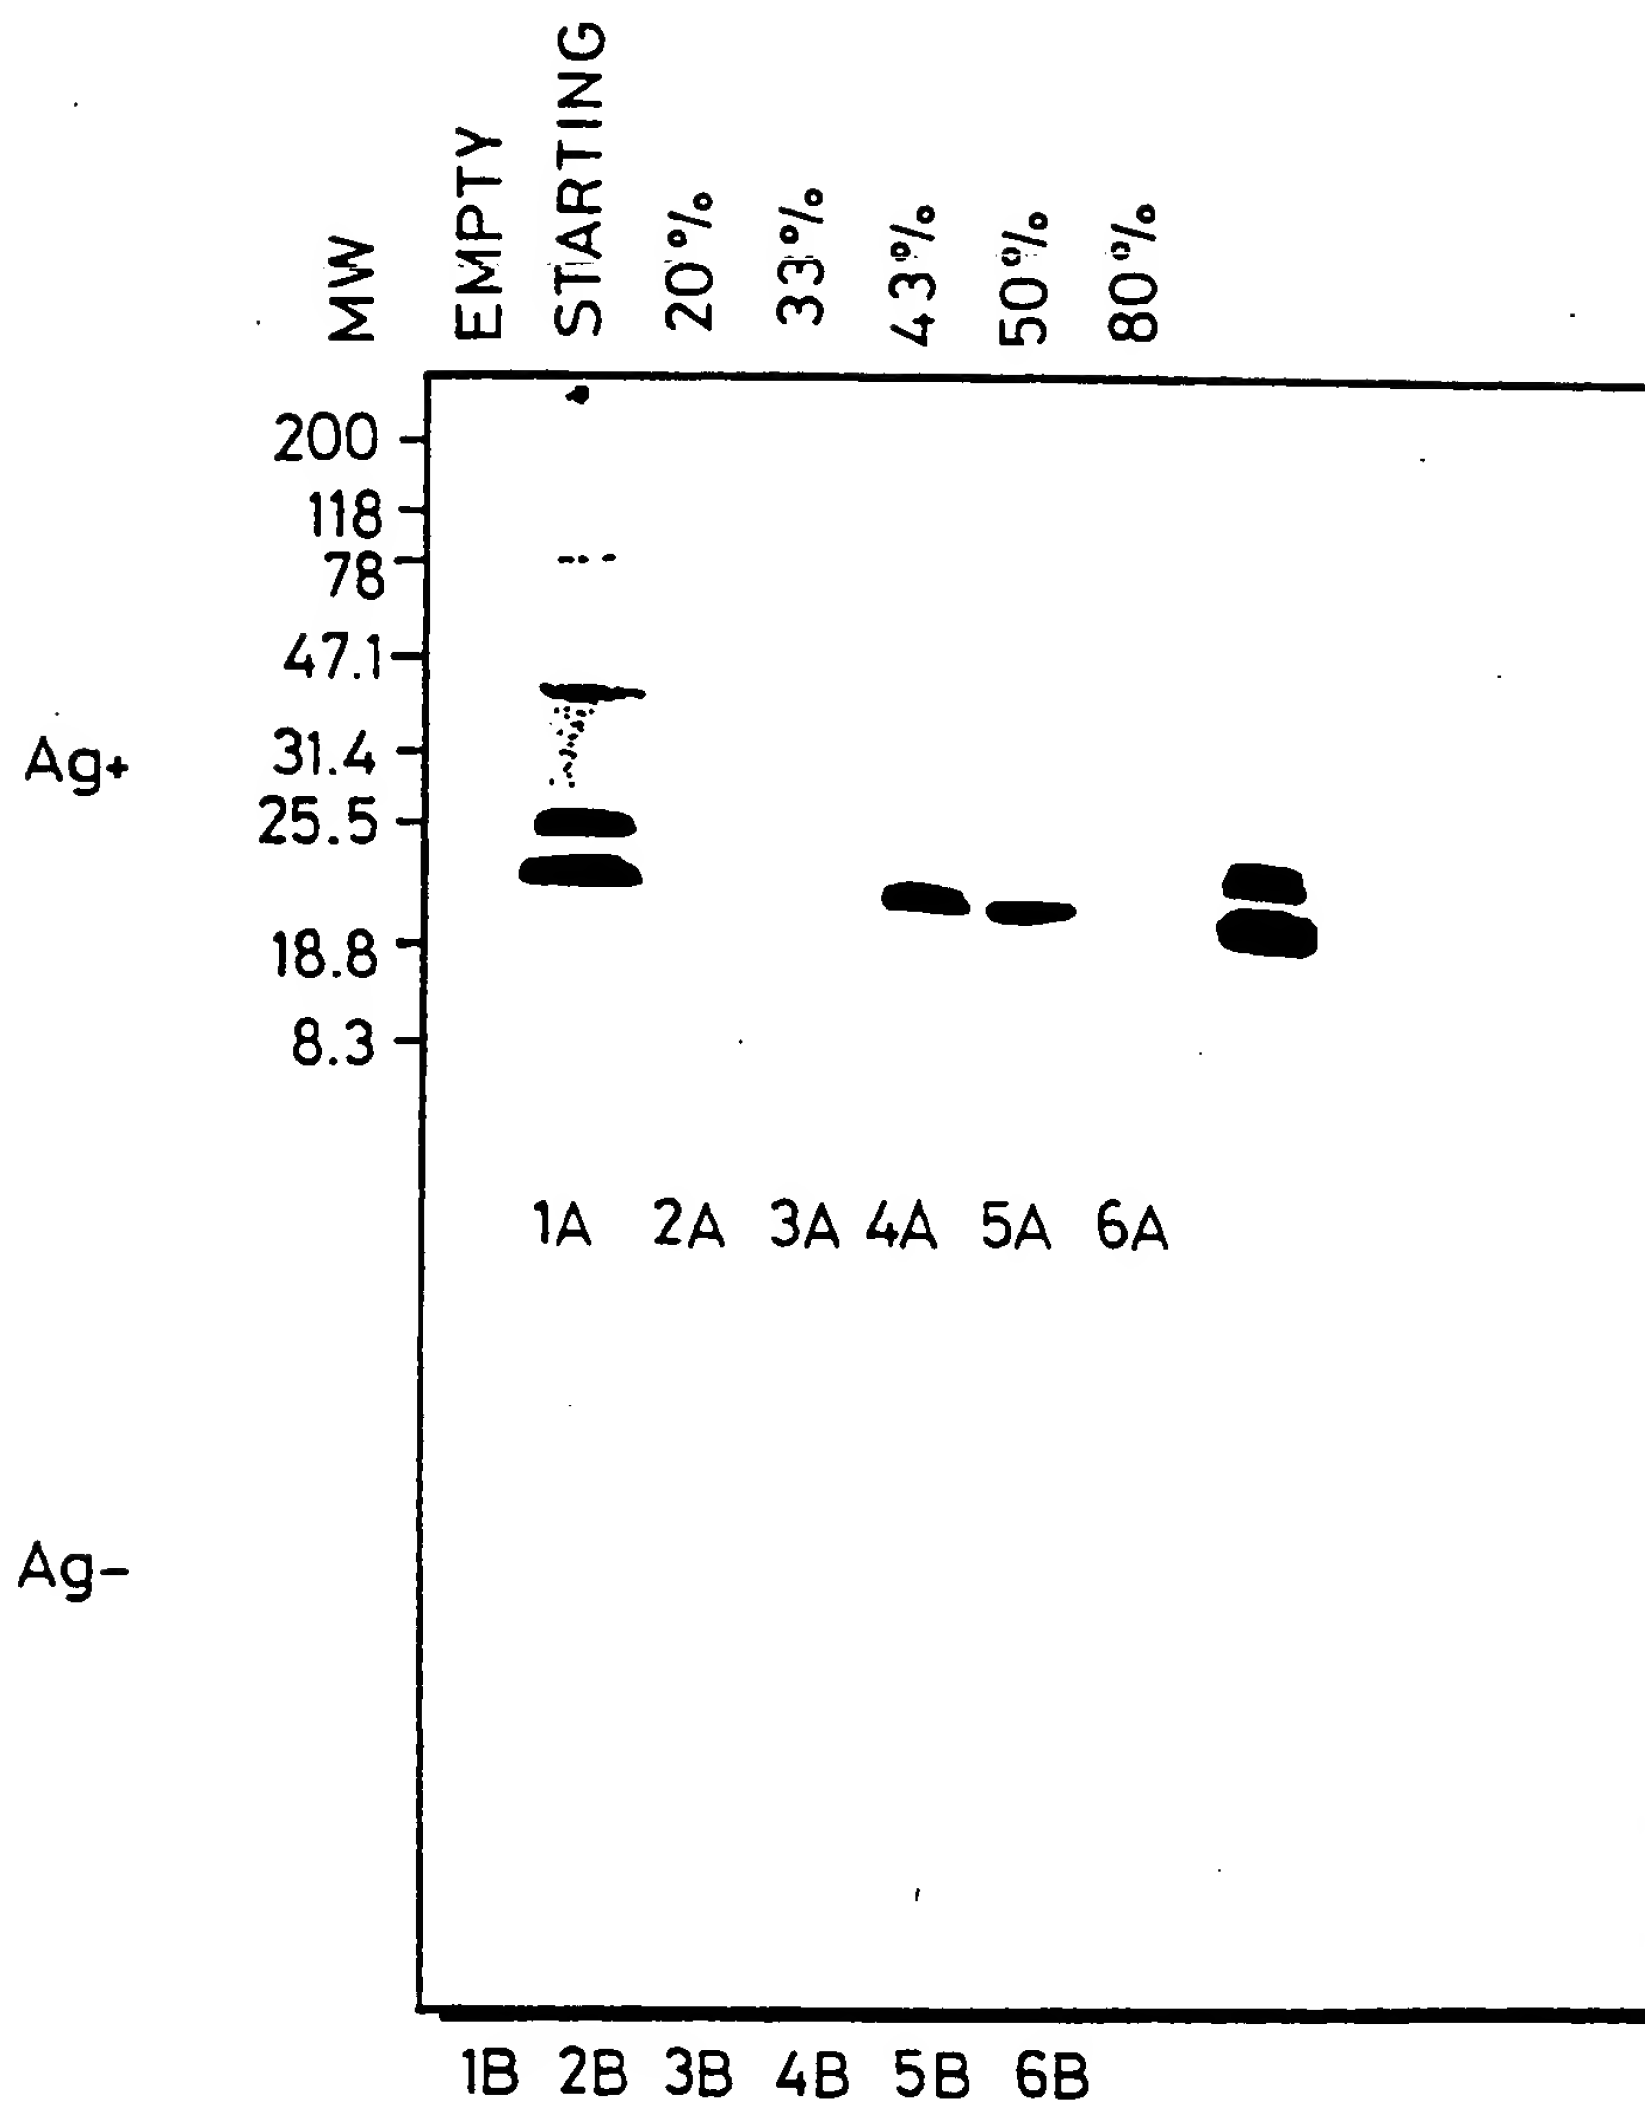

14/14

FIG. 13

